
Photovoltaic devices –

Part 8:

Guidance for the measurement of spectral response
of a photovoltaic (PV) device

Dispositifs photovoltaïques –

*Partie 8: Guide pour le mesurage de la réponse spectrale
d'un dispositif photovoltaïque (PV)*

Validité de la présente publication

Le contenu technique des publications de la CEI est constamment revu par la CEI afin qu'il reflète l'état actuel de la technique

Des renseignements relatifs à la date de reconfirmation de la publication sont disponibles auprès du Bureau Central de la CEI

Les renseignements relatifs à ces révisions, à l'établissement des éditions révisées et aux amendements peuvent être obtenus auprès des Comités nationaux de la CEI et dans les documents ci-dessous

- **Bulletin de la CEI**
- **Annuaire de la CEI**
Publié annuellement
- **Catalogue des publications de la CEI**
Publié annuellement et mis à jour régulièrement

Terminologie

En ce qui concerne la terminologie générale, le lecteur se reportera à la CEI 50: *Vocabulaire Electrotechnique International* (VEI), qui se présente sous forme de chapitres séparés traitant chacun d'un sujet défini. Des détails complets sur le VEI peuvent être obtenus sur demande. Voir également le dictionnaire multilingue de la CEI

Les termes et définitions figurant dans la présente publication ont été soit tirés du VEI, soit spécifiquement approuvés aux fins de cette publication.

Symboles graphiques et littéraux

Pour les symboles graphiques, les symboles littéraux et les signes d'usage général approuvés par la CEI, le lecteur consultera

- la CEI 27 *Symboles littéraux à utiliser en électrotechnique*,
- la CEI 417 *Symboles graphiques utilisables sur le matériel. Index, relevé et compilation des feuilles individuelles*,
- la CEI 617 *Symboles graphiques pour schémas*,

et pour les appareils électromédicaux,

- la CEI 878 *Symboles graphiques pour équipements électriques en pratique médicale*.

Les symboles et signes contenus dans la présente publication ont été soit tirés de la CEI 27, de la CEI 417, de la CEI 617 et/ou de la CEI 878, soit spécifiquement approuvés aux fins de cette publication.

Publications de la CEI établies par le même comité d'études

L'attention du lecteur est attirée sur les listes figurant à la fin de cette publication, qui énumèrent les publications de la CEI préparées par le comité d'études qui a établi la présente publication

Validity of this publication

The technical content of IEC publications is kept under constant review by the IEC, thus ensuring that the content reflects current technology

Information relating to the date of the reconfirmation of the publication is available from the IEC Central Office

Information on the revision work, the issue of revised editions and amendments may be obtained from IEC National Committees and from the following IEC sources:

- **IEC Bulletin**
- **IEC Yearbook**
Published yearly
- **Catalogue of IEC publications**
Published yearly with regular updates

Terminology

For general terminology, readers are referred to IEC 50: *International Electrotechnical Vocabulary (IEV)*, which is issued in the form of separate chapters each dealing with a specific field. Full details of the IEV will be supplied on request. See also the IEC Multilingual Dictionary

The terms and definitions contained in the present publication have either been taken from the IEV or have been specifically approved for the purpose of this publication

Graphical and letter symbols

For graphical symbols, and letter symbols and signs approved by the IEC for general use, readers are referred to publications:

- IEC 27 *Letter symbols to be used in electrical technology*,
- IEC 417 *Graphical symbols for use on equipment. Index, survey and compilation of the single sheets*,
- IEC 617: *Graphical symbols for diagrams*,

and for medical electrical equipment,

- IEC 878: *Graphical symbols for electromedical equipment in medical practice*.

The symbols and signs contained in the present publication have either been taken from IEC 27, IEC 417, IEC 617 and/or IEC 878, or have been specifically approved for the purpose of this publication

IEC publications prepared by the same technical committee

The attention of readers is drawn to the end pages of this publication which list the IEC publications issued by the technical committee which has prepared the present publication.

INTERNATIONAL STANDARD

IEC
904-8

First edition
1995-09

Photovoltaic devices –

Part 8:

Guidance for the measurement of spectral response
of a photovoltaic (PV) device

Dispositifs photovoltaïques –

*Partie 8. Guide pour le mesurage de la réponse spectrale
d'un dispositif photovoltaïque (PV)*

© CEI 1995 Droits de reproduction réservés — Copyright — all rights reserved

Aucune partie de cette publication ne peut être reproduite ni
utilisée sous quelque forme que ce soit et par aucun pro-
cédé électronique ou mécanique, y compris la photocopie et
les microfilms sans l'accord écrit de l'éditeur

No part of this publication may be reproduced or utilized in
any form or by any means electronic or mechanical,
including photocopying and microfilm, without permission
in writing from the publisher

Bureau Central de la Commission Electrotechnique Internationale 3, rue de Varembé Genève, Suisse



Commission Electrotechnique Internationale
International Electrotechnical Commission
Международная Электротехническая Комиссия

INTERNATIONAL ELECTROTECHNICAL COMMISSION

PHOTOVOLTAIC DEVICES –

**Part 8: Guidance for the measurement of spectral response
of a photovoltaic (PV) device**

FOREWORD

- 1) The IEC (International Electrotechnical Commission) is a worldwide organization for standardization comprising all national electrotechnical committees (IEC National Committees). The object of the IEC is to promote international co-operation on all questions concerning standardization in the electrical and electronic fields. To this end and in addition to other activities, the IEC publishes International Standards. Their preparation is entrusted to technical committees, any IEC National Committee interested in the subject dealt with may participate in this preparatory work. International, governmental and non-governmental organizations liaising with the IEC also participate in this preparation. The IEC collaborates closely with the International Organization for Standardization (ISO) in accordance with conditions determined by agreement between the two organizations.
- 2) The formal decisions or agreements of the IEC on technical matters, prepared by technical committees on which all the National Committees having a special interest therein are represented, express as nearly as possible, an international consensus of opinion on the subjects dealt with.
- 3) They have the form of recommendations for international use published in the form of standards, technical reports or guides and they are accepted by the National Committees in that sense.
- 4) In order to promote international unification, IEC National Committees undertake to apply IEC International Standards transparently to the maximum extent possible in their national and regional standards. Any divergence between the IEC Standard and the corresponding national or regional standard shall be clearly indicated in the latter.
- 5) The IEC provides no marking procedure to indicate its approval and cannot be rendered responsible for any equipment declared to be in conformity with one of its standards.

International Standard IEC 904-8 has been prepared by IEC technical committee 82: Solar photovoltaic energy systems.

The text of this standard is based on the following documents:

DIS	Report on voting
82(CO)14	82(CO)21

Full information on the voting for the approval of this standard can be found in the report on voting indicated in the above table.

PHOTOVOLTAIC DEVICES –

Part 8: Guidance for the measurement of spectral response of a photovoltaic (PV) device

1 Scope

This part of IEC 904 gives guidance for the measurement of the relative spectral response of both linear and non-linear photovoltaic devices.

2 Normative references

The following normative documents contain provisions which, through reference in this text, constitute provisions of this part of IEC 904. At the time of publication, the editions indicated were valid. All normative documents are subject to revision, and parties to agreements based on this part of IEC 904 are encouraged to investigate the possibility of applying the most recent editions of the normative documents indicated below. Members of IEC and ISO maintain registers of currently valid International Standards.

IEC 904-1: 1987, *Photovoltaic devices – Part 1: Measurement of photovoltaic current-voltage characteristics*

IEC 904-2: 1989, *Photovoltaic devices – Part 2: Requirements for reference solar cells*

IEC 904-3: 1989, *Photovoltaic devices – Part 3: Measurement principles for terrestrial photovoltaic (PV) solar devices with reference spectral irradiance data*

3 Relative spectral response measurement

The relative spectral response of a photovoltaic (PV) device is measured by irradiating it by means of a narrow-bandwidth light source at a series of different wavelengths covering its response range, and measuring the short-circuit current density and irradiance at each of these wavelengths.

NOTE – In this standard, the words "light" and "sunlight" are used in their broader sense to include the ultra-violet and the infra-red as well as the visible spectrum

The light source should irradiate the device uniformly and the temperature of the device should be controlled. The current densities are then divided by the irradiances or a proportional parameter and plotted as a function of wavelength. Alternatively, the irradiance may be kept constant (for instance, by varying the length of a monochromator exit slit), in which case the relative spectral response is obtained directly from the current density readings.

The irradiance monitor may be a vacuum thermocouple, a pyroelectric radiometer or other suitable detector. Another alternative is a previously calibrated reference photovoltaic device whose relative spectral response covers the required range. In this case, the relative spectral response of the test specimen is computed as follows:

$$k_2 \cdot s_{2\lambda} = k_1 \cdot s_{1\lambda} \frac{J_{m1\lambda}}{J_{m2\lambda}}$$

where

$k_1 \cdot S_{1\lambda}$ is the relative spectral response of the reference photovoltaic device at wavelength λ ;

$k_2 \cdot S_{2\lambda}$ is the relative spectral response of the test specimen at the same wavelength;

$J_{mr\lambda}$ is the measured short-circuit current density of the reference photovoltaic device at wavelength λ ;

$J_{mt\lambda}$ is the measured short-circuit current density of the test specimen at the same wavelength.

In assembling the test set-up and performing the measuring, special attention should be given to the following:

- Uniformity of irradiance at the test plane (uniform irradiance is very important when test specimen and reference photovoltaic devices are of different dimensions).
- Filter transmission curves should be checked periodically to detect any "harmonic" transmission.
- Load resistor calibration and contact resistance should be checked.
- Linearity of response of the short-circuit current of the device versus the light intensity at all illumination levels and all wavelengths.
- The load resistor should be kept to a minimum practical value in order to remain as close as possible to true short-circuit conditions.

Figures 1 and 2 show two examples of test arrangements, the first embodying a quartz prism monochromator and the second a filter wheel as the monochromatic source.

NOTE - In this standard the word "monochromatic" is used to mean narrow bandwidth

In both cases, the light source is a 1 000 W tungsten halogen lamp operated from a stable supply at a colour temperature of 3 200 K. The test cell and the irradiance monitor are mounted on opposite sides of a rotatable temperature-controlled block, so that either may be presented to the monochromatic beam in precisely the same place. Alternatively, they may be mounted on a slide with suitable positioning stops, or illuminated simultaneously by means of a beam splitter

The filter wheel should contain a sufficient number of narrow-band filters to cover the response range of the cell in wavelength steps not exceeding 50 nm. The filters are arranged so that each can be indexed in turn between the light source and the test cell or irradiance monitor. It is important that the filters should have negligible (under 0,2 %) side-bands. The monochromator is normally used with fixed slits and manually set to the same wavelength steps.

With crystalline silicon and other cells where the response has been shown to change linearly with irradiance, the short-circuit current of the cells (voltage drop across a standard 4-terminal fixed resistor) and the open-circuit voltage of the vacuum thermocouple or radiometer may be measured directly with a d.c. digital voltmeter or potentiometer. The requirements for instrumentation accuracy and the measurement of short-circuit currents given in IEC 904-1 and IEC 904-3 apply. If the d.c. method is used, the exit beam, test specimen and irradiance monitor should be completely enclosed in an anti-reflective light-tight box and meticulous precautions should be taken to avoid thermal and random electro-magnetic fields which would cause errors. Alternatively, the exit beam may be chopped at a low frequency and the output voltages amplified and rectified. In this case, it is important to ensure that the amplifiers are linear and drift-free.

With non-linear devices it is necessary to use a chopped monochromatic beam, and to increase the irradiance to the desired operational level (e.g., $1\,000\text{ W m}^{-2}$) using unmodulated bias light from a suitable steady-state simulator as shown in figures 1 and 2. For linear devices the bias light is also necessary unless there is proof that the obtained spectral response will not change significantly when the bias light is not used.

A method for pulsed solar spectral response measurements is shown in figure 3. Apart from the change of light source, the measurement method remains the same, and is based on the comparison of the short-circuit currents generated by the cell to be measured and by the spectrally calibrated reference device. The test set-up comprises:

- a powerful flash lamp which provides high intensity light pulses;
- a filter wheel and light-tight box as previously described;
- a sample holder that ensures reproducible positioning of the test specimen and the reference photovoltaic device;
- reference photovoltaic device(s) spectrally calibrated in accordance with IEC 904-2 (specialized radiometry laboratories are best equipped to perform this calibration);
- a decade load resistor;
- an electronic “peak-detector”;
- a digital voltmeter.

NOTE – The pulsed light method cannot be used on test specimens whose response time is too slow. Therefore, it must be verified that the same short-circuit current density is obtained from pulsed and steady-state light sources having the same intensity. This same requirement also applies to the reference device.

In assembling the test set-up and in performing the measurements, special attention should be given to the light pulse intensity monitoring and the subsequent reading correction which may either be manual or, better, automatic.

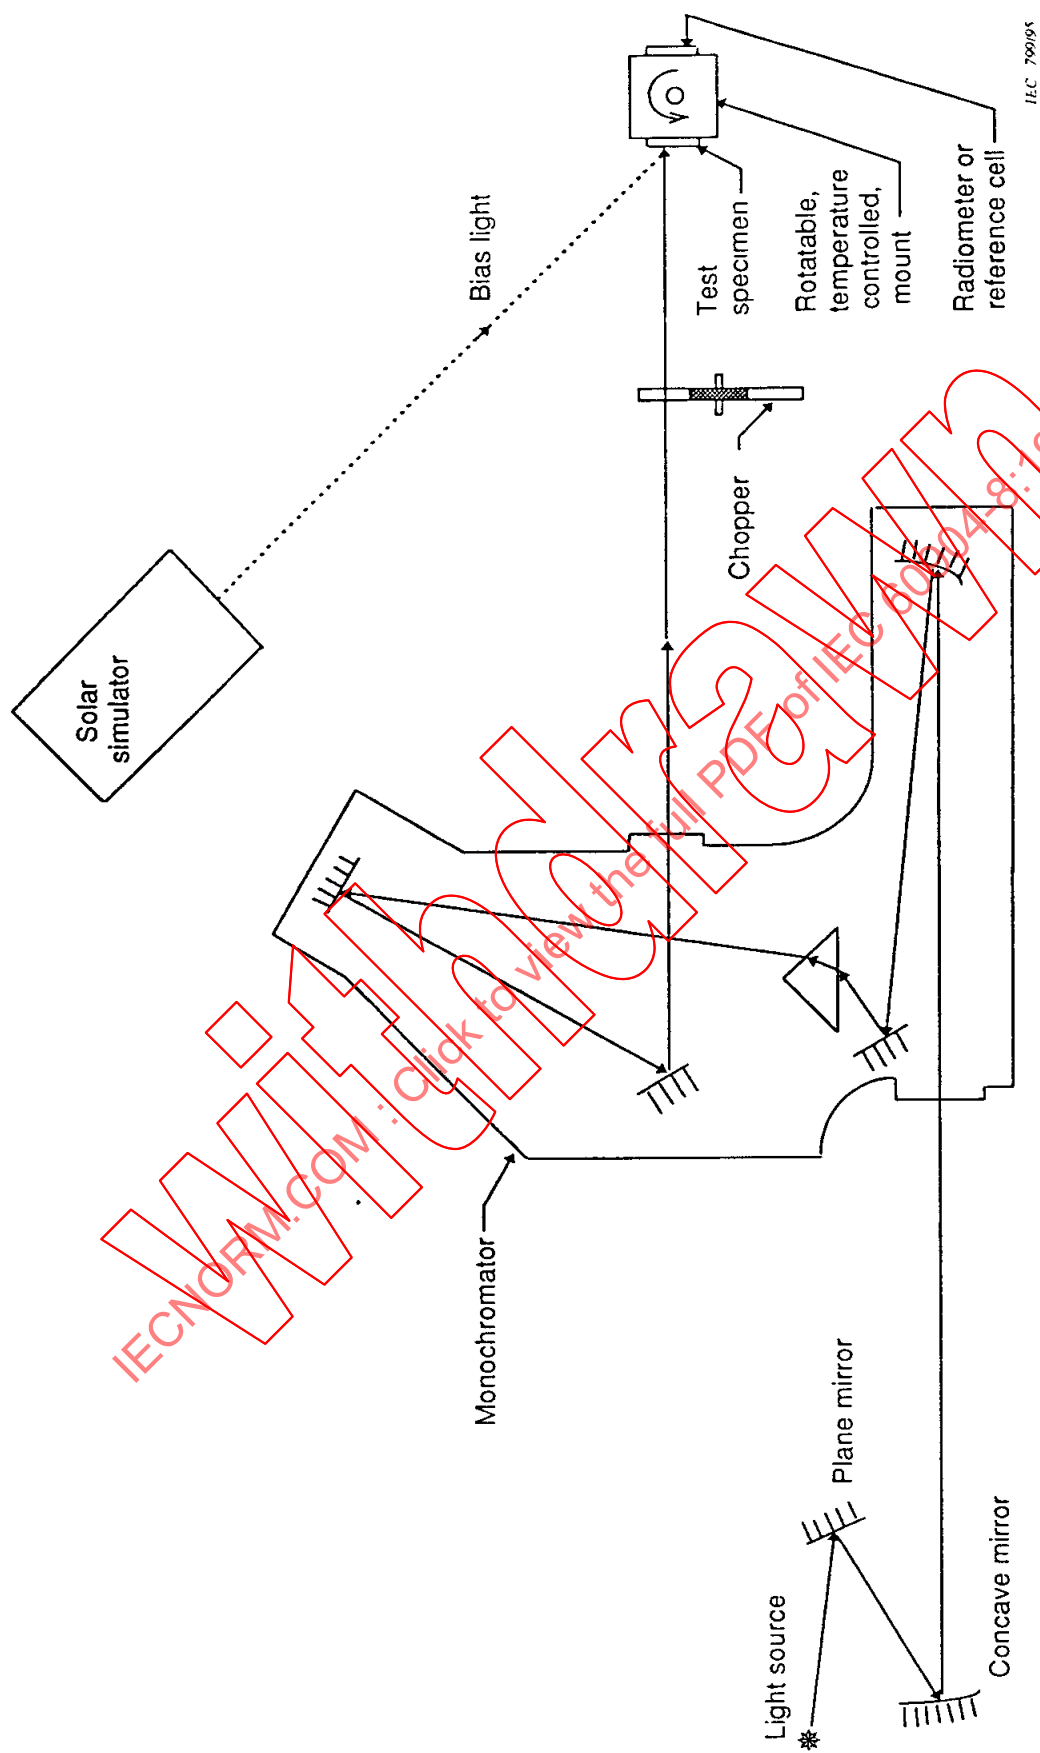


Figure 1 – Spectral response measurement using a monochromator

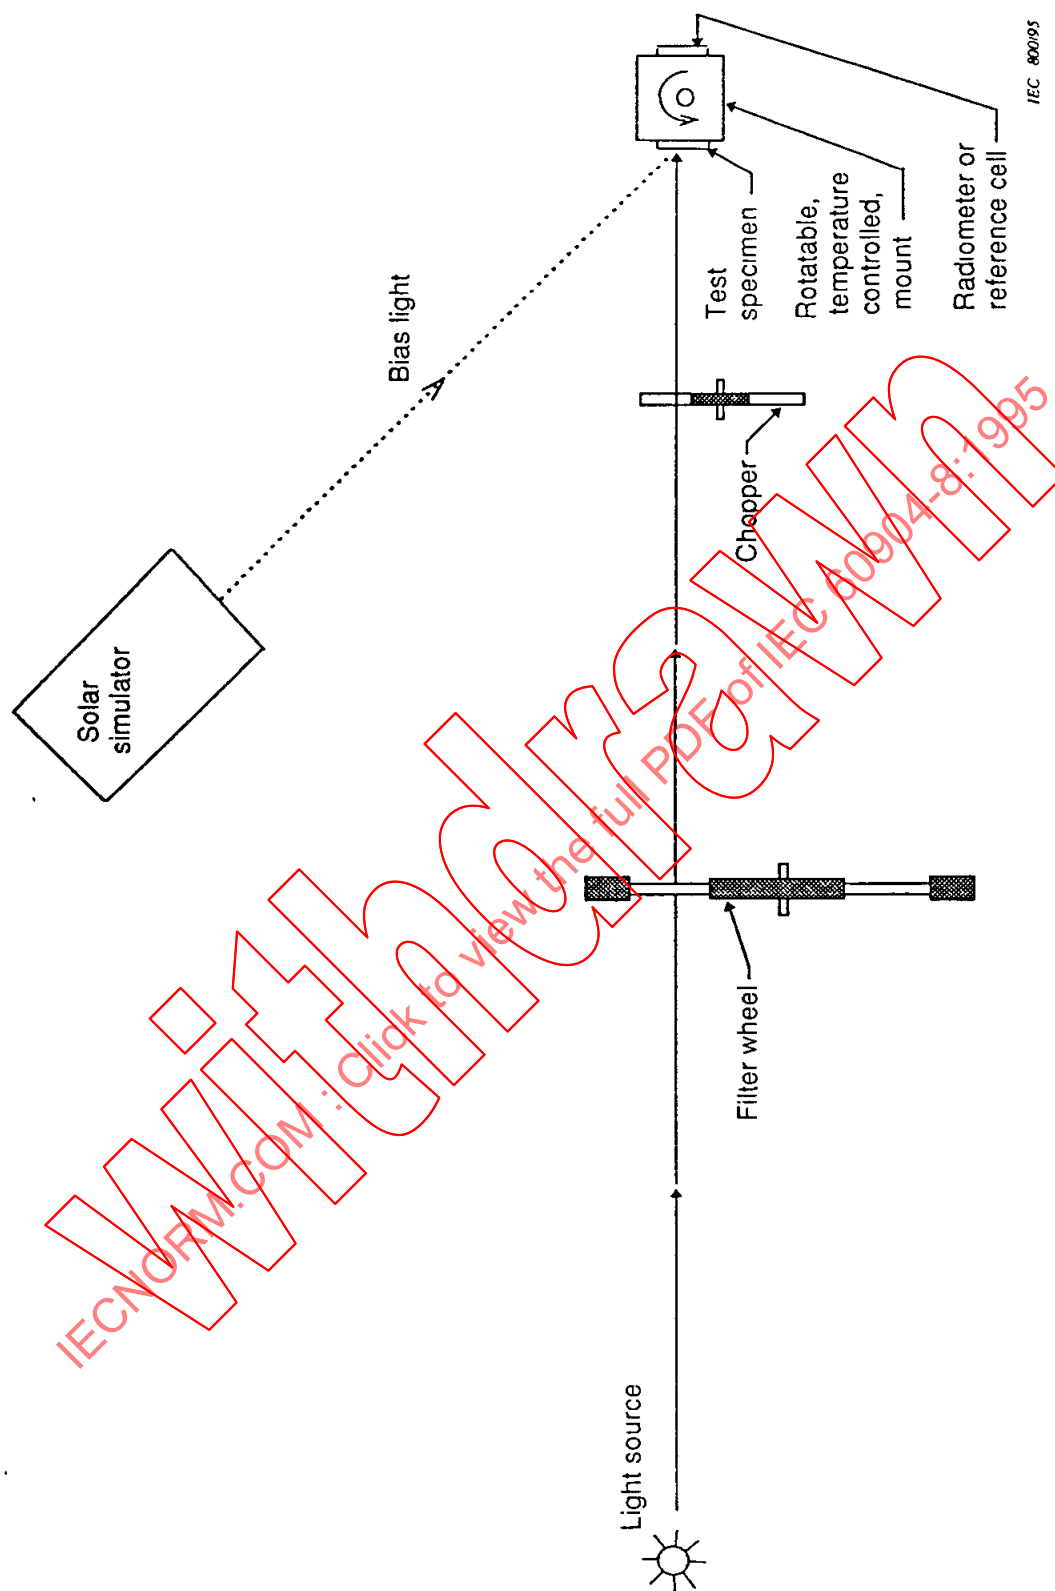


Figure 2 – Spectral response measurement using a filter wheel