

NFPA® 270

Standard Test Method for Measurement of Smoke Obscuration Using a Conical Radiant Source in a Single Closed Chamber

2023 Edition



NFPA, 1 Batterymarch Park, Quincy, MA 02169-7471
An International Codes and Standards Organization

IMPORTANT NOTICES AND DISCLAIMERS CONCERNING NFPA® STANDARDS

NFPA® codes, standards, recommended practices, and guides (“NFPA Standards”), of which the document contained herein is one, are developed through a consensus standards development process approved by the American National Standards Institute. This process brings together volunteers representing varied viewpoints and interests to achieve consensus on fire and other safety issues. While the NFPA administers the process and establishes rules to promote fairness in the development of consensus, it does not independently test, evaluate, or verify the accuracy of any information or the soundness of any judgments contained in NFPA Standards.

The NFPA disclaims liability for any personal injury, property, or other damages of any nature whatsoever, whether special, indirect, consequential or compensatory, directly or indirectly resulting from the publication, use of, or reliance on NFPA Standards. The NFPA also makes no guaranty or warranty as to the accuracy or completeness of any information published herein.

In issuing and making NFPA Standards available, the NFPA is not undertaking to render professional or other services for or on behalf of any person or entity. Nor is the NFPA undertaking to perform any duty owed by any person or entity to someone else. Anyone using this document should rely on his or her own independent judgment or, as appropriate, seek the advice of a competent professional in determining the exercise of reasonable care in any given circumstances.

The NFPA has no power, nor does it undertake, to police or enforce compliance with the contents of NFPA Standards. Nor does the NFPA list, certify, test, or inspect products, designs, or installations for compliance with this document. Any certification or other statement of compliance with the requirements of this document shall not be attributable to the NFPA and is solely the responsibility of the certifier or maker of the statement.

REVISION SYMBOLS IDENTIFYING CHANGES FROM THE PREVIOUS EDITION

Text revisions are shaded. A **Δ** before a section number indicates that words within that section were deleted and a **Δ** to the left of a table or figure number indicates a revision to an existing table or figure. When a chapter was heavily revised, the entire chapter is marked throughout with the **Δ** symbol. Where one or more sections were deleted, a **•** is placed between the remaining sections. Chapters, annexes, sections, figures, and tables that are new are indicated with an **N**.

Note that these indicators are a guide. Rearrangement of sections may not be captured in the markup, but users can view complete revision details in the First and Second Draft Reports located in the archived revision information section of each code at www.nfpa.org/docinfo. Any subsequent changes from the NFPA Technical Meeting, Tentative Interim Amendments, and Errata are also located there.

REMINDER: UPDATING OF NFPA STANDARDS

Users of NFPA codes, standards, recommended practices, and guides (“NFPA Standards”) should be aware that these documents may be superseded at any time by the issuance of a new edition, may be amended with the issuance of Tentative Interim Amendments (TIAs), or be corrected by Errata. It is intended that through regular revisions and amendments, participants in the NFPA standards development process consider the then-current and available information on incidents, materials, technologies, innovations, and methods as these develop over time and that NFPA Standards reflect this consideration. Therefore, any previous edition of this document no longer represents the current NFPA Standard on the subject matter addressed. NFPA encourages the use of the most current edition of any NFPA Standard [as it may be amended by TIA(s) or Errata] to take advantage of current experience and understanding. An official NFPA Standard at any point in time consists of the current edition of the document, including any issued TIAs and Errata then in effect.

To determine whether an NFPA Standard has been amended through the issuance of TIAs or corrected by Errata, visit the “Codes & Standards” section at www.nfpa.org.

ADDITIONAL IMPORTANT NOTICES AND DISCLAIMERS CONCERNING NFPA® STANDARDS

Updating of NFPA Standards

Users of NFPA codes, standards, recommended practices, and guides (“NFPA Standards”) should be aware that these documents may be superseded at any time by the issuance of a new edition, may be amended with the issuance of Tentative Interim Amendments (TIAs), or be corrected by Errata. It is intended that through regular revisions and amendments, participants in the NFPA standards development process consider the then-current and available information on incidents, materials, technologies, innovations, and methods as these develop over time and that NFPA Standards reflect this consideration. Therefore, any previous edition of this document no longer represents the current NFPA Standard on the subject matter addressed. NFPA encourages the use of the most current edition of any NFPA Standard [as it may be amended by TIA(s) or Errata] to take advantage of current experience and understanding. An official NFPA Standard at any point in time consists of the current edition of the document, including any issued TIAs and Errata then in effect.

To determine whether an NFPA Standard has been amended through the issuance of TIAs or corrected by Errata, visit the “Codes & Standards” section at www.nfpa.org.

Interpretations of NFPA Standards

A statement, written or oral, that is not processed in accordance with Section 6 of the Regulations Governing the Development of NFPA Standards shall not be considered the official position of NFPA or any of its Committees and shall not be considered to be, nor be relied upon as, a Formal Interpretation.

Patents

The NFPA does not take any position with respect to the validity of any patent rights referenced in, related to, or asserted in connection with an NFPA Standard. The users of NFPA Standards bear the sole responsibility for determining the validity of any such patent rights, as well as the risk of infringement of such rights, and the NFPA disclaims liability for the infringement of any patent resulting from the use of or reliance on NFPA Standards.

NFPA adheres to the policy of the American National Standards Institute (ANSI) regarding the inclusion of patents in American National Standards (“the ANSI Patent Policy”), and hereby gives the following notice pursuant to that policy:

NOTICE: The user’s attention is called to the possibility that compliance with an NFPA Standard may require use of an invention covered by patent rights. NFPA takes no position as to the validity of any such patent rights or as to whether such patent rights constitute or include essential patent claims under the ANSI Patent Policy. If, in connection with the ANSI Patent Policy, a patent holder has filed a statement of willingness to grant licenses under these rights on reasonable and nondiscriminatory terms and conditions to applicants desiring to obtain such a license, copies of such filed statements can be obtained, on request, from NFPA. For further information, contact the NFPA at the address listed below.

Law and Regulations

Users of NFPA Standards should consult applicable federal, state, and local laws and regulations. NFPA does not, by the publication of its codes, standards, recommended practices, and guides, intend to urge action that is not in compliance with applicable laws, and these documents may not be construed as doing so.

Copyrights

NFPA Standards are copyrighted. They are made available for a wide variety of both public and private uses. These include both use, by reference, in laws and regulations, and use in private self-regulation, standardization, and the promotion of safe practices and methods. By making these documents available for use and adoption by public authorities and private users, the NFPA does not waive any rights in copyright to these documents.

Use of NFPA Standards for regulatory purposes should be accomplished through adoption by reference. The term “adoption by reference” means the citing of title, edition, and publishing information only. Any deletions, additions, and changes desired by the adopting authority should be noted separately in the adopting instrument. In order to assist NFPA in following the uses made of its documents, adopting authorities are requested to notify the NFPA (Attention: Secretary, Standards Council) in writing of such use. For technical assistance and questions concerning adoption of NFPA Standards, contact NFPA at the address below.

For Further Information

All questions or other communications relating to NFPA Standards and all requests for information on NFPA procedures governing its codes and standards development process, including information on the procedures for requesting Formal Interpretations, for proposing Tentative Interim Amendments, and for proposing revisions to NFPA standards during regular revision cycles, should be sent to NFPA headquarters, addressed to the attention of the Secretary, Standards Council, NFPA, 1 Batterymarch Park, P.O. Box 9101, Quincy, MA 02269-9101; email: stds_admin@nfpa.org.

For more information about NFPA, visit the NFPA website at www.nfpa.org. All NFPA codes and standards can be viewed at no cost at www.nfpa.org/docinfo.

Copyright © 2022 National Fire Protection Association®. All Rights Reserved.

NFPA® 270

Standard Test Method for

Measurement of Smoke Obscuration Using a Conical Radiant Source in a Single Closed Chamber

2023 Edition

This edition of NFPA 270, *Standard Test Method for Measurement of Smoke Obscuration Using a Conical Radiant Source in a Single Closed Chamber*, was prepared by the Technical Committee on Fire Tests. It was issued by the Standards Council on November 29, 2022, with an effective date of December 19, 2022, and supersedes all previous editions.

This edition of NFPA 270 was approved as an American National Standard on December 19, 2022.

Origin and Development of NFPA 270

The first edition of this standard, the 1998 edition, was based on the 1997 edition of NFPA 258, *Standard Research Test Method for Determining Smoke Generation of Solid Materials*, with minor revisions. Originally, NFPA 258 was used for research and product development. NFPA 270 was developed so that it could be used within the regulatory community for enforcement purposes. This document was developed under a different title and number designation so as not to confuse the end user and to establish and clarify the intention and limitations that are now part of the standard.

The 2002 edition of this standard was updated to incorporate the *Manual of Style for NFPA Technical Committee Documents* requirements and editorial updates.

The 2008 edition of this standard contained mainly editorial revisions and revised definitions for consistency with other standards.

The 2013 edition of this standard reconfirmed of the previous edition and updated the referenced standards.

The 2018 edition of NFPA 270 included updates to the pressure sensor requirements to reflect modern technology and updated the referenced codes and standards.

The 2023 edition includes revisions to improve consistency with ASTM E1995 and updates to referenced standards.

Technical Committee on Fire Tests

Barry L. Badders, Jr., Chair
Intertek Testing Services, TX [RT]

Hubert Biteau, S-E-A, Ltd., CO [SE]
Benjamin H. Caldwell, Skidmore, Owings & Merrill LLP (SOM), NY [SE]
Karen C. Carpenter, Southwest Research Institute, TX [RT]
Rick D. Davis, National Institute of Standards & Technology (NIST), MD [RT]
Scott E. Dillon, Crane Engineering, MN [SE]
William E. Fitch, Phyrefish.com, FL [SE]
Richard G. Gann, Gaithersburg, MD [SE]
Marcelo M. Hirschler, GBH International, CA [SE]
Paul A. Hough, Armstrong World Industries, Inc., PA [M]
William E. Koffel, Koffel Associates, Inc., MD [SE]
Sergei V. Levchik, Israel Chemicals Ltd. (ICL-IP), NY [M]
Rep. ACC-North American Flame Retardant Alliance
Michael E. Luna, ICC NTA, LLC., TX [RT]
James Andrew Lynch, The Fire Solutions Group, PA [SE]
John Martell, Professional Fire Fighters of Maine/IAFF, ME [L]
Rep. International Association of Fire Fighters

Rodney A. McPhee, Canadian Wood Council, Canada [M]
Kathleen A. Newman, Firetect, CA [M]
Nicholas Ozog, Wiss, Janney, Elstner Associates, Inc., IL [SE]
Arthur J. Parker, JENSEN HUGHES, MD [SE]
Bill Perdue, American Home Furnishings Alliance (AHFA), NC [U]
Shamim Rashid-Sumar, National Ready Mixed Concrete Assn., NY [M]
Michael L. Savage, Sr., Marion County Building Safety, FL [E]
Michael Schmeida, Gypsum Association, OH [M]
David T. Sheppard, US Bureau of Alcohol, Tobacco, Firearms & Explosives, MD [RT]
Dwayne Sloan, UL LLC, NC [RT]
Kuma Sumathipala, American Wood Council, VA [M]
Robert J. Wills, American Iron and Steel Institute, AL [M]
Dong Zeng, FM Global, MA [I]
Rep. FM Global

Alternates

Marc Alam, Canadian Wood Council, Canada [M]
(Alt. to Rodney A. McPhee)
Richard J. Davis, FM Global, MA [I]
(Alt. to Dong Zeng)
Timothy Earl, GBH International, MI [SE]
(Alt. to Marcelo M. Hirschler)
Stephen Paul Fuss, US Bureau of Alcohol, Tobacco, Firearms & Explosives, MD [RT]
(Alt. to David T. Sheppard)
Justin A. Geiman, Fire and Risk Alliance LLC, MD [SE]
(Alt. to James Andrew Lynch)
Karl Dana Houser, Intertek, PA [RT]
(Alt. to Barry L. Badders, Jr.)
Jonathan Humble, American Iron and Steel Institute, CT [M]
(Alt. to Robert J. Wills)

Marc L. Janssens, Southwest Research Institute, TX [RT]
(Alt. to Karen C. Carpenter)
Elizabeth C. Keller, Engineering Systems, Inc., NC [SE]
(Alt. to Scott E. Dillon)
Cori Leffler, Firetect, CA [M]
(Alt. to Kathleen A. Newman)
Daniel A. Martin, JENSEN HUGHES, MD [SE]
(Alt. to Arthur J. Parker)
Jason V. Smart, American Wood Council (AWC), VA [M]
(Alt. to Kuma Sumathipala)
Matthew T. Vinci, International Association of Fire Fighters, DC [L]
(Alt. to John Martell)
Luke C. Woods, UL LLC, MA [RT]
(Alt. to Dwayne Sloan)

Nonvoting

Rohit “Rik” Khanna, US Consumer Product Safety Commission (CPSC), MD [C]
Rep. US Consumer Product Safety Commission

Andrew Lock, US Consumer Product Safety Commission, MD [C]
Rep. US Consumer Product Safety Commission

Tracy L. Vecchiarelli, NFPA Staff Liaison

This list represents the membership at the time the Committee was balloted on the final text of this edition. Since that time, changes in the membership may have occurred. A key to classifications is found at the back of the document.

NOTE: Membership on a committee shall not in and of itself constitute an endorsement of the Association or any document developed by the committee on which the member serves.

Committee Scope: This Committee shall have primary responsibility for documents on fire testing procedures, for reviewing existing fire test standards and recommending appropriate action to NFPA, for recommending the application of and advising on the interpretation of acceptable test standards for fire problems of concern to NFPA technical committees and members, and for acting in a liaison capacity between NFPA and the committees of other organizations writing fire test standards. This Committee does not cover fire tests that are used to evaluate extinguishing agents, devices, or systems.

Contents

Chapter 1 Administration	270– 4	7.3 Selection of Compensating Filter(s).	270– 13
1.1 Scope.	270– 4	7.4 Linearity Check.	270– 14
1.2 Purpose. (Reserved)	270– 4	7.5 Calibration of Range-Extension Filter.	270– 14
1.3 Application.	270– 4	7.6 Chamber Leakage Rate Test.	270– 14
1.4 Units and Formulas.	270– 5	7.7 Burner Calibration.	270– 14
Chapter 2 Referenced Publications	270– 5	7.8 Radiator Cone Calibration.	270– 14
2.1 General.	270– 5	7.9 Cleaning.	270– 15
2.2 NFPA Publications. (Reserved)	270– 5	7.10 Frequency of Checking and Calibrating Procedures.	270– 15
2.3 Other Publications.	270– 5	7.11 Total System.	270– 16
2.4 References for Extracts in Mandatory Sections. (Reserved)	270– 6	Chapter 8 Conditioning	270– 16
Chapter 3 Definitions	270– 6	8.1 Pre-Test.	270– 16
3.1 General.	270– 6	8.2 Conditioning.	270– 16
3.2 NFPA Official Definitions.	270– 6	Chapter 9 Test Procedure	270– 16
3.3 General Definitions.	270– 6	9.1 Initial Conditions.	270– 16
Chapter 4 Test Apparatus	270– 6	9.2 Tests with Pilot Flame.	270– 16
4.1 General.	270– 6	9.3 Preparation of Photometric System.	270– 16
4.2 Test Chamber.	270– 6	9.4 Loading Specimen.	270– 16
4.3 Sample Support and Heating Arrangements. ...	270– 7	9.5 Recording of Light Transmission.	270– 16
4.4 Gas Supply.	270– 9	9.6 Observations.	270– 16
4.5 Photometric System.	270– 10	9.7 Termination of Test.	270– 17
4.6 Chamber Leakage.	270– 11	9.8 Specimen Mass.	270– 17
4.7 Cleaning Materials.	270– 11	9.9 Repeat Tests.	270– 17
4.8 Ancillary Equipment.	270– 11	Chapter 10 Calculations	270– 17
Chapter 5 Test Environment	270– 11	10.1 Specific Optical Density, D_s	270– 17
5.1 Light Interference.	270– 11	10.2 Clear Beam Correction Factor, D_c	270– 18
5.2 Product of Combustion Venting.	270– 11	10.3 Mass Loss.	270– 18
5.3 Operator Safety.	270– 11	Chapter 11 Test Report	270– 18
Chapter 6 Test Specimen	270– 12	11.1 Descriptive Information.	270– 18
6.1 Suitability of Sample for Testing.	270– 12	11.2 Test Results.	270– 18
6.2 Sample Face.	270– 12	Annex A Explanatory Material	270– 18
6.3 Number of Specimens.	270– 12	Annex B Precision and Bias	270– 21
6.4 Additional Specimens.	270– 12	Annex C Interlaboratory Application	270– 24
6.5 Size of Specimens.	270– 12	Annex D Determination of Mass Optical Density	270– 25
6.6 Specimen Preparation.	270– 12	Annex E Informational References	270– 30
6.7 Wrapping of Specimens.	270– 13	Index	270– 32
Chapter 7 Setup, Calibration, and Maintenance	270– 13		
7.1 Setup and Calibration Procedures.	270– 13		
7.2 Alignment of Photometric System.	270– 13		

NFPA 270

Standard Test Method for

Measurement of Smoke Obscuration Using a Conical Radiant Source in a Single Closed Chamber

2023 Edition

IMPORTANT NOTE: This NFPA document is made available for use subject to important notices and legal disclaimers. These notices and disclaimers appear in all publications containing this document and may be found under the heading “Important Notices and Disclaimers Concerning NFPA Standards.” They can also be viewed at www.nfpa.org/disclaimers or obtained on request from NFPA.

UPDATES, ALERTS, AND FUTURE EDITIONS: New editions of NFPA codes, standards, recommended practices, and guides (i.e., NFPA Standards) are released on scheduled revision cycles. This edition may be superseded by a later one, or it may be amended outside of its scheduled revision cycle through the issuance of Tentative Interim Amendments (TIAs). An official NFPA Standard at any point in time consists of the current edition of the document, together with all TIAs and Errata in effect. To verify that this document is the current edition or to determine if it has been amended by TIAs or Errata, please consult the National Fire Codes® Subscription Service or the “List of NFPA Codes & Standards” at www.nfpa.org/docinfo. In addition to TIAs and Errata, the document information pages also include the option to sign up for alerts for individual documents and to be involved in the development of the next edition.

NOTICE: An asterisk (*) following the number or letter designating a paragraph indicates that explanatory material on the paragraph can be found in Annex A.

A reference in brackets [] following a section or paragraph indicates material that has been extracted from another NFPA document. Extracted text may be edited for consistency and style and may include the revision of internal paragraph references and other references as appropriate. Requests for interpretations or revisions of extracted text shall be sent to the technical committee responsible for the source document.

Information on referenced and extracted publications can be found in Chapter 2 and Annex E.

Chapter 1 Administration

1.1 Scope.

1.1.1 This is a fire-test-response standard.

1.1.2* This test method provides a means of measuring smoke obscuration resulting from subjecting essentially flat materials, products, or assemblies (including surface finishes) not exceeding 25 mm in thickness to specified levels of thermal irradiance from a conical heater, in a single closed chamber, in the absence or presence of a pilot flame, and when placed in a horizontal orientation.

1.1.3 The principal fire-test-response characteristic obtained from this test method shall be the specific optical density of smoke from the specimens tested, which is obtained as a function of time, for a period of 10 minutes.

1.1.4 Other fire-test-response characteristics are also permitted to be determined.

1.1.5 An optional fire-test-response characteristic measurable with this test method shall be the mass optical density, which is the specific optical density of smoke divided by the mass lost by the specimens during the test.

1.1.6 The fire-test-response characteristics obtained from this test are specific to the specimen tested, in the form and thickness tested, and are not inherent properties of the material, product, or assembly tested.

1.1.7* This test method does not provide information on the fire performance of the test specimens under fire conditions other than those conditions specified in this test method.

1.1.8 This standard measures and describes the response of materials, products, or assemblies to heat and flame under controlled conditions but does not by itself incorporate all factors required for fire hazard or fire risk assessment of the materials, products, or assemblies under actual fire conditions.

1.1.9* Fire testing of products and materials is inherently hazardous, and safeguards for personnel and property shall be employed in conducting these tests.

1.1.10 This standard does not purport to address all of the safety problems, if any, associated with its use.

1.1.11 It shall be the responsibility of the user of this standard to establish the necessary safety and health practices and determine the applicability of regulatory limitations prior to use.

1.2 Purpose. (Reserved)

1.3 Application.

1.3.1 Summary of Test Method.

1.3.1.1 Energy Source.

1.3.1.1.1 This test method shall employ a conically shaped, electrically heated radiant energy source contained within a stainless steel tube and positioned so as to produce an irradiance level of up to 50 kW/m², averaged over the center of the exposed surface of an essentially flat specimen, mounted horizontally, to determine smoke obscuration inside a closed chamber.

1.3.1.1.2 The actual irradiance levels used for standard testing shall be 25 kW/m² and 50 kW/m².

1.3.1.2 Specimen. The specimen shall be 75 mm × 75 mm at a thickness not exceeding 25 mm and shall be mounted horizontally within a holder.

1.3.1.3 Pilot Flame.

1.3.1.3.1 The exposure shall be conducted in the absence or in the presence of a pilot flame as described in 4.3.6.1.

1.3.1.3.2 Where the pilot flame is present, the test shall be deemed to be in the “flaming” mode; if the pilot flame is absent, the test shall be deemed to be in the “nonflaming” mode.

1.3.1.4 Light Transmissions.

1.3.1.4.1 The test specimens shall be exposed to nonflaming or flaming conditions within a closed chamber.

1.3.1.4.2 A photometric system with a vertical light path shall be used to measure the varying light transmission as smoke accumulates.

1.3.1.4.3 The light transmittance measurements shall be used to calculate the specific optical density of the smoke generated during the test.

1.3.1.5 Exposure.

1.3.1.5.1 The specimens shall be exposed to two conditions out of the four standard exposure conditions, to be chosen by the test requester.

1.3.1.5.2 The four standard exposure conditions shall be as follows:

- (1) Flaming at an irradiance of 25 kW/m²
- (2) Flaming at an irradiance of 50 kW/m²
- (3) Nonflaming at an irradiance of 25 kW/m²
- (4) Nonflaming at an irradiance of 50 kW/m²

1.3.1.5.3 The default conditions for testing, unless specified otherwise, shall be those in the flaming mode.

1.3.1.5.4 Exposures to other irradiances shall also be permitted.

1.3.1.6* Mass Optical Density. Mass optical density shall be an optional fire-test-response characteristic obtained from this test method by using a load cell that continuously monitors the mass of the test specimen.

1.3.2 Significance and Use.

1.3.2.1* Specific Optical Density.

1.3.2.1.1 This test method shall provide a means for determining the specific optical density of the smoke generated by specimens of materials, products, or assemblies under the specified exposure conditions.

1.3.2.1.2 Values determined by this test method shall be specific to the specimen in the form and thickness tested and shall not be inherent fundamental properties of the material, product, or assembly.

1.3.2.1.3 Closely repeatable or reproducible experimental results shall not be expected from this test method when tests are conducted for a given material, product, or assembly while introducing variations in properties such as specimen thickness or density.

1.3.2.2* Physiological Aspects. Physiological aspects associated with vision shall not be measured by this test method.

1.3.2.3* Smoke Obscuration. Predicting the smoke obscuration to be generated by the specimens upon exposure to heat or flame under any fire conditions other than those specified shall not be permitted.

1.3.3 Limitations.

1.3.3.1 Behavior. Any of the following behaviors during a test shall render that test invalid:

- (1) Self-ignition in the nonflaming mode
- (2) A specimen being displaced from the zone of controlled irradiance so as to touch the pilot burner or the pilot flame
- (3) Extinction of the pilot flame (even for a short period of time) in the flaming mode
- (4) Molten material overflowing the specimen holder

1.3.3.2* Data Evaluation. Evaluation of the data obtained, together with the individual masses, shall assist in assessing the reasons for any observed variation in measurements.

1.3.3.3* Sample Thickness. The results of the test shall apply only to the thickness of the sample being tested.

1.3.3.4* Sensitivity. Sensitivity to variations shall require that when changing to another sample to be tested, it shall first be necessary to clean and remove from the walls all accumulated residues to ensure that chemical or physical recombination with the effluents or residues produced as a result of the thermal irradiance does not affect the data obtained.

1.3.3.5* Test Conditions. Specimens shall be subjected to one or more specific sets of laboratory test conditions.

1.3.3.5.1 The results shall be valid only for the fire-test-exposure conditions described in this test.

1.3.3.5.2 This test method shall not be used to predict changes in the fire-test-response characteristics where different test conditions are substituted or end-use conditions are changed.

1.3.3.6* Optical Density. Information relating the specific optical density measurement obtained by this test method to the mass lost by the specimen during the test shall be obtained only by using the (optional) load cell to determine the mass optical density.

1.3.3.7* Dynamic Measurements. This test method shall not use dynamic measurements.

1.3.3.8 Smoke Obscuration. Therefore, the smoke obscuration values obtained shall not represent conditions of open fires.

1.4 Units and Formulas. The values stated in SI units shall be considered the required values of this standard.

Chapter 2 Referenced Publications

2.1 General. The documents or portions thereof listed in this chapter are referenced within this standard and shall be considered part of the requirements of this document.

2.2 NFPA Publications. (Reserved)

2.3 Other Publications.

2.3.1 ANSI Publications. American National Standards Institute, Inc., 25 West 43rd Street, 4th Floor, New York, NY 10036.

ANSI/AHA A135.4, *Basic Hardboard*, 2020.

2.3.2 ASTM Publications. ASTM International, 100 Barr Harbor Drive, P.O. Box C700, West Conshohocken, PA 19428-2959.

ASTM C1186, *Standard Specification for Flat Fiber-Cement Sheets*, 2008 (2016).

ASTM C1288, *Standard Specification for Fiber-Cement Interior Substrate Sheets*, 2017.

ASTM E176, *Standard Terminology of Fire Standards*, 2021a.

▲ **2.3.3 ISO Publications.** International Organization for Standardization, ISO Central Secretariat, BIBC II, Chemin de Blandonnet 8, CP 401, 1214 Vernier, Geneva, Switzerland.

ISO 13943, *Fire safety — Vocabulary*, 2017.

2.3.4 Other Publications.

Merriam-Webster's Collegiate Dictionary, 11th edition, Merriam-Webster, Inc., Springfield, MA, 2003.

2.4 References for Extracts in Mandatory Sections. (Reserved)

Chapter 3 Definitions

3.1 General. The definitions contained in this chapter shall apply to the terms used in this standard. Where terms are not defined in this chapter or within another chapter, they shall be defined using their ordinarily accepted meanings within the context in which they are used. *Merriam-Webster's Collegiate Dictionary*, 11th edition, shall be the source for the ordinarily accepted meaning.

3.2 NFPA Official Definitions.

3.2.1 Shall. Indicates a mandatory requirement.

3.2.2 Standard. An NFPA standard, the main text of which contains only mandatory provisions using the word “shall” to indicate requirements and that is in a form generally suitable for mandatory reference by another standard or code or for adoption into law. Nonmandatory provisions are not to be considered a part of the requirements of a standard and shall be located in an appendix, annex, footnote, informational note, or other means as permitted in the NFPA manuals of style. When used in a generic sense, such as in the phrases “standards development process” or “standards development activities,” the term “standards” includes all NFPA standards, including codes, standards, recommended practices, and guides.

3.3 General Definitions. For definitions of terms used in this test method, refer to the terminology contained in ASTM E176, *Standard Terminology of Fire Standards*, and ISO 13943, *Fire safety — Vocabulary*.

3.3.1 Assembly. A unit or structure composed of a combination of materials or products, or both.

3.3.2 Composite. A combination of materials that are generally recognized as distinct entities, for example, coated or laminated materials.

3.3.3 Continuous (as related to data acquisition). Conducted at data collection intervals of 5 seconds or less.

3.3.4 Exposed Surface. That surface of the specimen subjected to the incident heat.

3.3.5 Mass Optical Density (MOD). The ratio of the optical density of smoke to the mass loss of the test specimen, multiplied by the volume of the test chamber and divided by the length of the light path.

3.3.6 Sample. An amount of the material, product, or assembly to be tested that is representative of the item as a whole.

3.3.7 Self-Ignition. The initiation of combustion as evidenced by the observed presence of flame.

3.3.8 Smoke Obscuration. The reduction of light transmission by smoke, as measured by light attenuation.

3.3.9 Time to Ignition. Time between the start of the test and the presence of a flame on or over most of the specimen surface for a period of at least 4 seconds.

Chapter 4 Test Apparatus

4.1 General. The apparatus shall consist of an airtight test chamber with provision for containing a sample holder, radiator cone, pilot burner, light transmission and measuring system, and other ancillary facilities for controlling the conditions of operation during a test as shown in Figure 4.1.

4.2 Test Chamber.

4.2.1 Fabrication. The test chamber shall be fabricated from laminated panels, the inner surfaces of which shall consist of either a porcelain-enameled metal not more than 1 mm thick or an equivalent coated metal that is resistant to chemical attack and corrosion and capable of being easily cleaned. (See Figure 4.1 and Figure 4.2.1.)

4.2.1.1 The internal dimensions of the chamber shall be 914 mm ± 3 mm long, 914 mm ± 3 mm high, as shown in Figure 4.2.1, and 610 mm ± 3 mm deep.

4.2.1.2 The chamber shall be provided with a hinged front-mounted door with an observation window and a removable opaque door cover to the window to prevent light from entering the chamber.

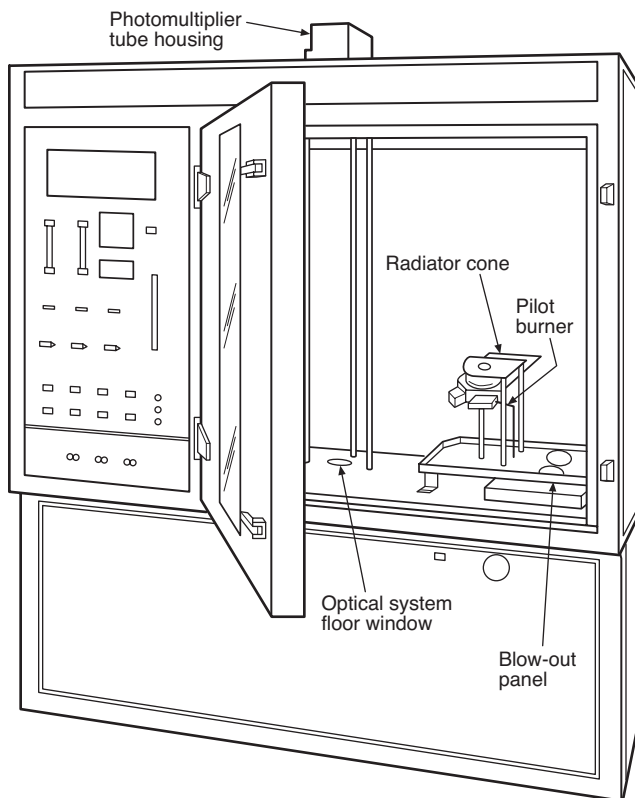


FIGURE 4.1 Typical Arrangement of Test Chamber.

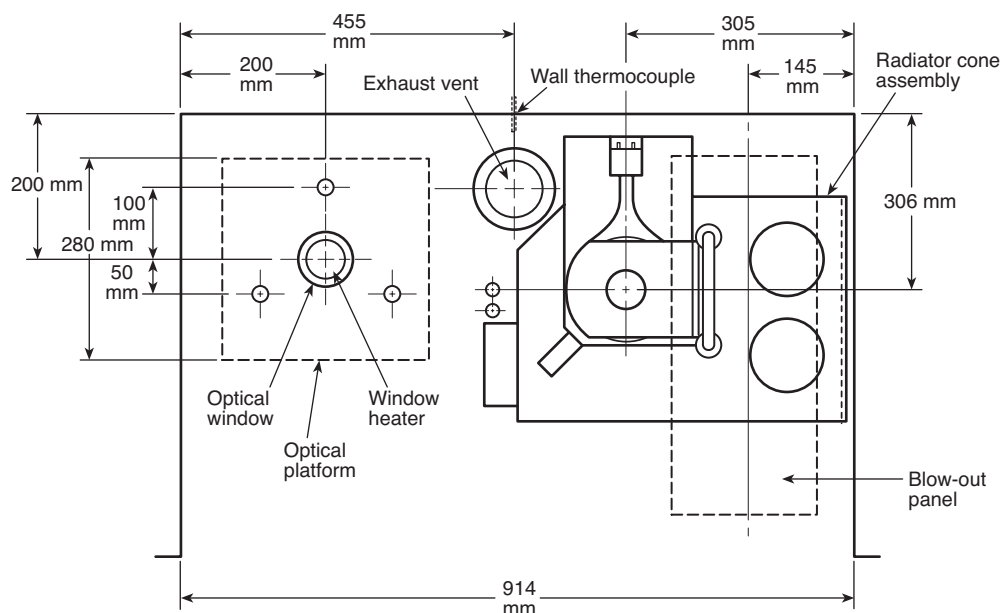


FIGURE 4.2.1 Plan View of Typical Test Chamber.

4.2.2* Panel. A safety blow-out panel consisting of a sheet of aluminum foil not greater than 0.04 mm thick and having a minimum area of 80,600 mm² shall be provided in the chamber, fastened in such a way as to provide an airtight seal.

4.2.3 Optical Windows.

4.2.3.1 Two optical windows, each with a diameter of 75 mm $\pm$ 1 mm, shall be mounted, one each in the top and the bottom of the cabinet, at the position shown in Figure 4.2.1, with their interior faces flush with the outside of the cabinet lining.

4.2.3.2* The underside of the window on the floor shall be provided with an electric heater of approximately 9 W capacity in the form of a ring, which shall be capable of maintaining the upper surface of the window at a temperature of at least 50°C and which shall be mounted around the window's edge so as not to interrupt the light path.

4.2.3.3 Optical platforms 8 mm $\pm$ 0.1 mm thick shall be mounted around the windows on the outside of the chamber and shall be held rigidly in position relative to each other by three metal rods, each with a diameter of at least 12.5 mm, extending through the chamber and fastened securely to the platforms.

4.2.4 Other Cabinet Openings.

4.2.4.1 Other openings in the cabinet shall be provided for the required services, as specified.

4.2.4.2 Cabinet openings shall be capable of being closed so that a positive pressure up to 1.5 kPa above atmospheric pressure can be developed inside the chamber as described in 4.2.6 and maintained when checked in accordance with Sections 4.6 and 7.6.

4.2.4.3 All components of the chamber shall be capable of withstanding a greater internal positive pressure than the safety blow-out panel.

4.2.5 Inlet Vent. An inlet vent with a shutter shall be provided at the top of the chamber, either on the front or on the roof,

and away from the radiator cone, and an exhaust vent with a shutter shall be provided in the bottom of the chamber to lead, via flexible pipe with a diameter of 50 mm to 100 mm, to an extraction fan capable of creating a negative pressure of at least 0.5 kPa.

4.2.6* Chamber Pressure Control Facilities.

4.2.6.1 Provision shall be made for controlling the pressure inside the test chamber.

4.2.6.2 A pressure sensor (such as a manometer or pressure transducer) with a range up to 5 kPa shall be provided to monitor chamber pressure and leakage.

4.2.7 Thermocouple Junction.

4.2.7.1 A thermocouple measuring junction made from wires of a diameter not greater than 1 mm shall be mounted on the inside of the back wall of the chamber, at the geometric center, by means of an insulating disc (such as polystyrene foam) that has a thickness of 6.5 mm $\pm$ 0.2 mm and a diameter of not more than 20 mm attached with an adhesive intended for such purposes.

4.2.7.2 The thermocouple junction shall be connected to a recorder, meter, or data acquisition unit, and the system shall be capable of measuring temperatures in the range of 35°C to 60°C as described in 9.1.3.3.

4.3 Sample Support and Heating Arrangements.

4.3.1 Radiator Cone.

4.3.1.1 Heating Element. The radiator cone, as shown in Figure 4.3.1.1, shall consist of a heating element of nominal rating 450 W contained within a stainless steel tube, 2210 mm $\pm$ 5 mm in length and 6.5 mm $\pm$ 0.2 mm in diameter, coiled into the shape of a truncated cone and fitted into a shade.

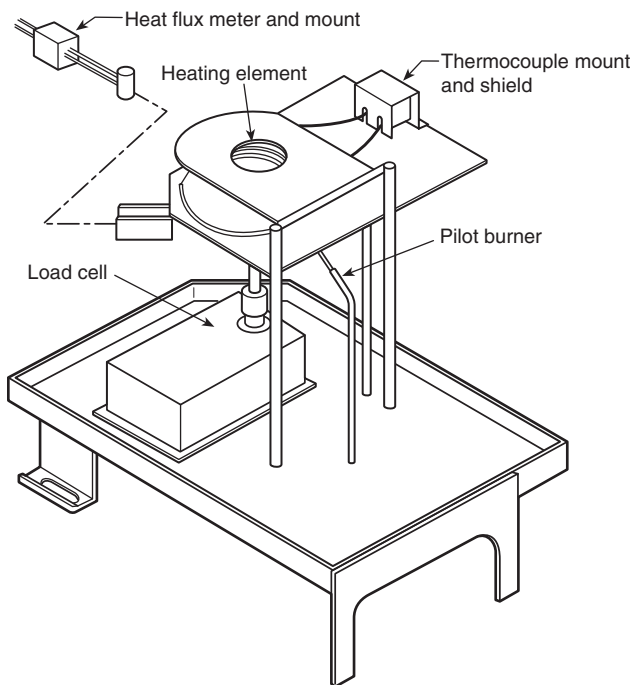


FIGURE 4.3.1.1 Typical Framework for Support of Radiator Cone, Specimen Holder, Flux Meter, and Load Cell.

4.3.1.1.1 The shade shall have an overall height of 45 mm $\pm$ 0.04 mm, an internal diameter of 55 mm $\pm$ 1 mm, and an internal base diameter of 110 mm $\pm$ 3 mm.

4.3.1.1.2 The shade shall consist of two layers of 1 mm $\pm$ 0.1 mm thick stainless steel with a 10 mm $\pm$ 0.5 mm thickness of ceramic fiber insulation of nominal density 100 kg/m³ sandwiched between them.

4.3.1.1.3 The heating element shall be clamped by two plates at the top and bottom of the element.

4.3.1.2 Radiator Cone Irradiance.

4.3.1.2.1 The radiator cone shall be capable of providing irradiance in the range of 10 to 50 kW/m² at the center of the surface of the specimen.

4.3.1.2.2 When the irradiance is determined at two other positions, 25 mm $\pm$ 2 mm each side of the specimen center, the irradiance at those two positions shall be not less than 85 percent or not more than 115 percent of the irradiance at the center of the specimen.

4.3.1.3* Irradiance Control.

4.3.1.3.1 The irradiance of the radiator cone shall be controlled by reference to the averaged reading of two Type K thermocouples.

4.3.1.3.2 The thermocouples shall have a 1.6 mm $\pm$ 0.2 mm outside diameter, sheathed with an unexposed hot junction; mounted diametrically opposite, in contact with, but not welded to, the heating element; and positioned at one-third the distance from the top surface of the cone.

4.3.1.4* Heater Temperature.

4.3.1.4.1 The temperature at the heater shall be controlled and shall be held steady to $\pm 2^\circ\text{C}$.

4.3.1.4.2 The temperature controller for the radiator cone shall be of the proportional, integral, and derivative type 3-term controller with thyristor stack fast-cycle or phase-angle control of not less than 10 A maximum rating.

4.3.1.4.3 Capacity for adjustment of integral time between 10 seconds and 50 seconds and differential time between 25 seconds and 30 seconds shall be provided to permit matching with the response characteristics of the heater.

4.3.1.4.4 The temperature input range shall be 0°C to 1000°C .

4.3.1.4.5 Automatic cold junction compensation of the thermocouple shall be provided.

4.3.1.4.6 Alternative devices that give equivalent results shall be permitted to be accepted.

4.3.2 Framework for Radiator Cone.

4.3.2.1 Vertical Rods. The radiator cone shall be secured to the vertical rods of the support framework and shall be located so that the lower rim of the radiator cone shade is 25 mm $\pm$ 1 mm above the upper surface of the specimen when oriented in the horizontal position as shown in Figure 4.3.2.1(a) and Figure 4.3.2.1(b).

4.3.2.2 Base. The base of the specimen holder shall contain a height adjustment device to ensure a consistent distance between the radiator cone and the specimen surface.

4.3.3 Radiator Shield.

4.3.3.1 Construction. The cone heater shall be provided with a removable radiator shield to protect the specimen from the irradiance prior to the start of the test.

4.3.3.1.1 The radiator shield shall be made of noncombustible material with a total thickness not to exceed 12 mm.

4.3.3.1.2 The radiator shield shall comply with one of the following:

- (1) A water-cooled radiator shield coated with a durable matte black finish of surface emissivity $\epsilon = 0.95 \pm 0.05$
- (2) A radiator shield with a metallic reflective top surface to minimize radiation transfer but not water cooled
- (3) A radiator shield with a ceramic, nonmetallic surface that minimizes radiation transfer to the specimen surface but not water cooled

4.3.3.2* Mobility. The radiator shield shall be equipped with a handle or other means for quick insertion and removal.

4.3.3.3 Stability. The cone heater base plate shall be equipped with the means for holding the radiator shield in position and allowing its quick removal.

4.3.4 Heat Flux Meter.

4.3.4.1* Target.

4.3.4.1.1 The heat flux meter shall be of the foil (Gardon) or thermopile (Schmidt-Boelter) type with a design range of at least 50 kW/m².

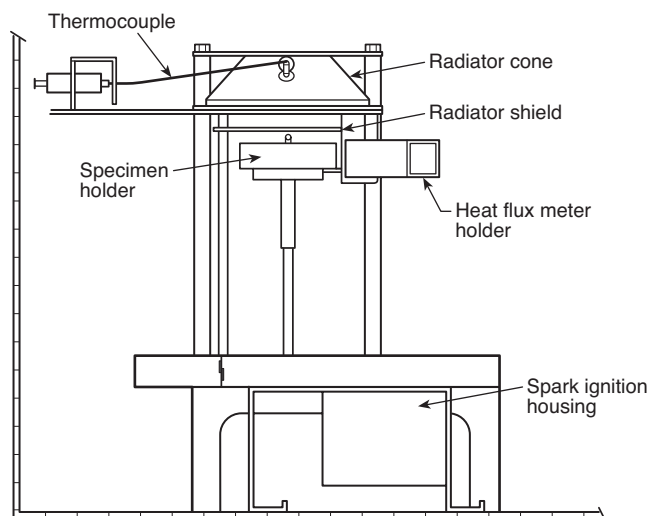


FIGURE 4.3.2.1(a) Typical Arrangement of Radiator Cone, Specimen Holder, and Radiator Shield (side view), with Load Cell for Mass Optical Density Determination.

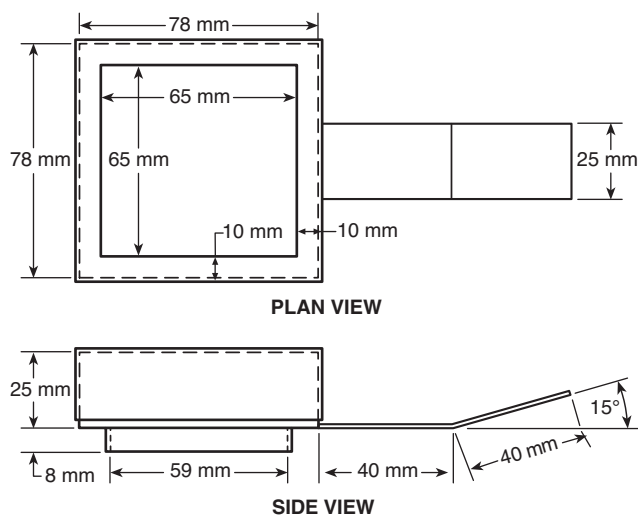


FIGURE 4.3.2.1(b) Specimen Holder.

4.3.4.1.2 The target receiving the radiation shall have a flat, circular face of $10 \text{ mm} \pm 1 \text{ mm}$ diameter, coated with a durable matte black finish.

4.3.4.1.3 The target shall be water cooled.

4.3.4.2* **Recorder.** The heat flux meter shall be connected directly to a recorder or data acquisition unit so that it is capable, when calibrated, of recording heat fluxes of 25 kW/m^2 and 50 kW/m^2 to an accuracy of $\pm 1 \text{ kW/m}^2$.

4.3.4.3 **Calibration.** The heat flux meter system shall be calibrated by comparing its response with that of a primary reference standard, when exposed to irradiances of 25 kW/m^2 and $50 \text{ kW/m}^2 \pm 1 \text{ kW/m}^2$, averaged over the $10 \text{ mm} \pm 1 \text{ mm}$ diameter area of the heat flux meter. (See Section B.1.)

4.3.5 Specimen Holders.

4.3.5.1 **Refractory Fiber Blanket.** The specimen holder base shall be lined with a low-density (nominal 65 kg/m^3) refractory fiber blanket with a minimum thickness of 10 mm as shown in Figure 4.3.2.1(b).

4.3.5.2 **Application.** Wrapped specimens less than 25 mm thick backed by at least one sheet of noncombustible insulating board shall be permitted to be used without a layer of refractory mineral fiber blanket if necessary to accommodate the specimens' thickness as described in 6.7.3.

4.3.5.3 Retainer Frame and Wire Grid.

4.3.5.3.1* A retainer frame and wire grid shall be used for all tests.

4.3.5.3.2 The wire grid shall be $75 \text{ mm} \pm 1 \text{ mm}$ square with $20 \text{ mm} \pm 0.5 \text{ mm}$ square holes constructed from $2 \text{ mm} \pm 0.2 \text{ mm}$ stainless steel rod welded at all intersections.

4.3.6* Pilot Burner.

4.3.6.1 **Flame.** The flame from the single-flame burner shall have a length of $30 \text{ mm} \pm 5 \text{ mm}$ and shall be positioned horizontally $10 \text{ mm} \pm 1 \text{ mm}$ above the top face of the specimen as shown in Figure 4.3.6.1.

4.3.6.2 **Color.** The color of the flame shall be blue with a yellow tip.

4.3.6.3 **Location.** The tip of the burner shall reach the edge of the specimen itself as shown in Figure 4.3.6.1.

4.4 Gas Supply.

4.4.1 A mixture of propane of at least 95 percent purity and at a pressure of $3.5 \text{ kPa} \pm 1 \text{ kPa}$ and air at a pressure of $170 \text{ kPa} \pm 30 \text{ kPa}$ shall be supplied to the burner.

4.4.2 Each gas shall be fed to the point at which they are mixed and supplied to the burner.

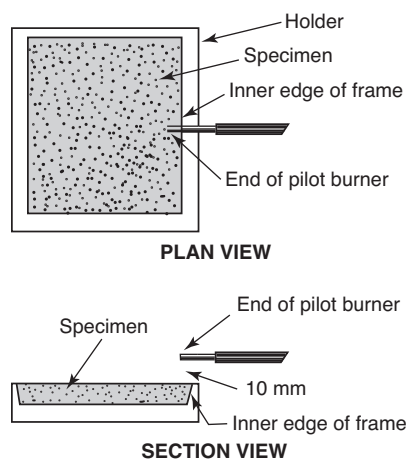


FIGURE 4.3.6.1 Detailed Location of Pilot Burner.

4.4.3 Needle valves and calibrated flowmeters shall be permitted to be used for controlling gas flows.

4.4.4 The flowmeter for the propane supply shall be capable of measuring 50 cm³/min flow rates.

4.4.5 The flowmeter for air supply shall be capable of measuring 500 cm³/min.

4.4.6 Alternative devices shown to give equivalent results shall also be permitted to be used.

4.5 Photometric System.

4.5.1 General.

4.5.1.1 Construction. The photometric system shall consist of a light source and lens in a lighttight housing mounted below the optical window in the floor of the cabinet and a photodetector with lens, filters, and a shutter in a lighttight housing above the optical window in the top of the chamber.

4.5.1.2 Equipment.

4.5.1.2.1 The system shall be as shown in Figure 4.5.1.2.1.

4.5.1.2.2 Equipment shall be provided to control the output of the light source and to measure the amount of light falling on the photodetector.

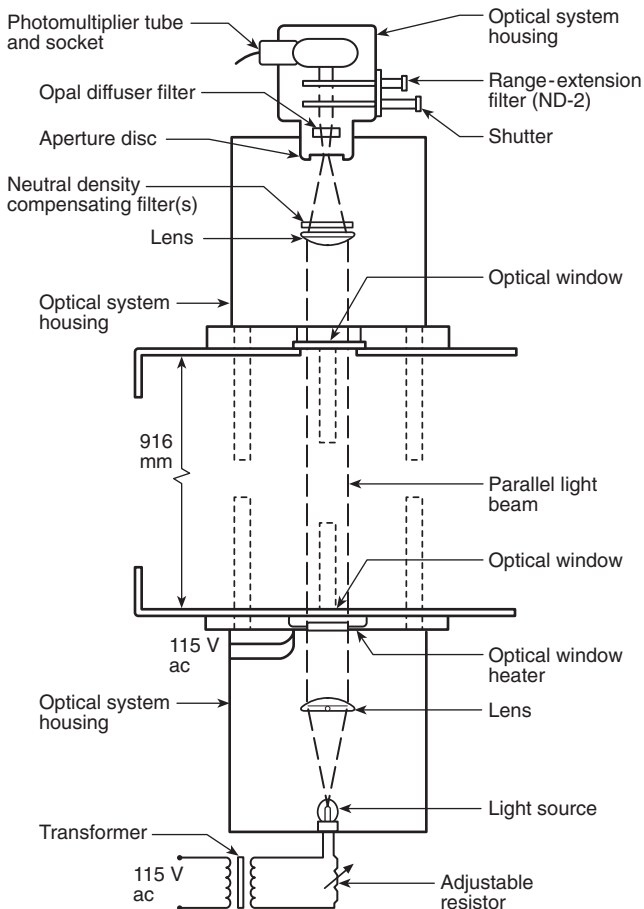


FIGURE 4.5.1.2.1 Photometric System.

4.5.2 Light Source.

4.5.2.1 The light source shall be a 6.5 V incandescent lamp.

4.5.2.2 Power for the lamp shall be provided by a transformer producing 6.5 V and a rheostat so that the voltage across the lamp as determined by an ac voltmeter is maintained at 4 V $\pm$ 0.2 V rms.

4.5.2.3 The lamp shall be mounted in the lower lighttight box, and a lens to provide a collimated light beam of 51 mm diameter passing toward and through the optical window on the floor of the chamber shall be mounted, with provision for adjustment, to control the collimated beam in direction and diameter.

4.5.2.4 The housing shall be provided with a cover to allow access for adjustments to be made to the position of the lens.

4.5.3 Photodetector.

4.5.3.1* Equipment. The light-measuring device system shall consist of a photomultiplier tube connected to a multirange amplifier coupled to a recording device or data acquisition unit as described in 4.8.6.

4.5.3.1.1 This system shall be capable of continuously measuring relative light intensity against time as percentage transmission over at least five orders of magnitude, with an S-4 spectral sensitivity response similar to that of human vision and a dark current less than 109 A.

4.5.3.1.2 The system shall have a linear response with respect to transmittance and an accuracy of better than ± 3 percent of the maximum reading on any range.

4.5.3.1.3 For selection of photomultiplier tubes, as applicable, the minimum sensitivity shall allow a 100 percent reading to be obtained with a 0.5 neutral density filter and an ND-2 range-extension filter as described in 4.5.3.2.2 in the light path.

4.5.3.1.4 Provision shall be made for adjusting the reading of the instrument under given conditions over the full range of any scale.

4.5.3.2 Photomultiplier Tube. The photomultiplier tube shall be mounted in the upper section of the photodetector housing.

4.5.3.2.1 Below the tube there shall be an assembly that provides for the rapid positioning of a filter and of a shutter, in or out of the path of the collimated light beam.

4.5.3.2.2 The filter, referred to as the range-extension filter (ND-2), shall be a glass neutral density filter of nominal optical density 2.

4.5.3.2.3 When in the closed position, the shutter shall prevent all light in the test chamber from reaching the photomultiplier tube.

4.5.3.2.4 An opal diffuser filter shall be permanently mounted below the shutter.

4.5.3.3 Lens. The lower part of the housing shall support a 51 mm $\pm$ 1 mm diameter lens capable of being adjusted, so that the collimated beam is focused to form a small intense spot of light at the disc aperture between the upper and lower parts of the housing.

4.5.3.3.1 Above the lens, there shall be a mount for supporting one or more compensating filters from a set of nine gelatin neutral density filters, with optical density varying from 0.1 to 0.9 in increments of 0.1.

4.5.3.3.2 The housing shall be provided with a cover to allow access for making adjustments to the position of the lens and for inserting or removing filters.

4.5.3.4* Filter Calibration. A neutral density filter with a nominal optical density of 3.0, large enough to cover the lower optical window, the actual optical density having been determined by calibration, shall be available for calibrating the photometric system.

4.5.4 Additional Equipment.

4.5.4.1 Template. A template for checking the collimated light beam shall consist of an opaque disc marked with a concentric ring of $51 \text{ mm} \pm 1 \text{ mm}$ diameter.

4.5.4.1.1 The template shall be capable of fitting snugly between the support pillars.

4.5.4.1.2 The template shall be capable of being attached to and centered on the underside of the upper optical window in the chamber.

4.5.4.2 Window Covering. A piece of white cloth or paper tissue or a neutral density filter of sufficient size to completely cover the lower optical window of the chamber and that is capable of transmitting an amount of light to give a midscale reading of the photometric system when switched to the scale with a range of 1 percent transmission shall be available for calibrating the range-extension filter.

4.5.4.3 Light Blocking. A piece of opaque material sufficiently large enough to cover the lower optical window shall be available for blocking the light from the light source entering the chamber.

4.6* Chamber Leakage. With the specified items of equipment assembled and ready for testing, the chamber shall comply with the requirements of the leakage rate test given in Section 7.6.

4.7* Cleaning Materials. The optical system windows, viewing windows, chamber walls, and specimen holders shall be cleaned regularly.

4.7.1* Optical System Windows. The exposed surfaces of the glass separating the photodetector and light-source housings from the interior of the chamber shall be cleaned after each test.

4.7.2 Viewing Window. The viewing window shall be cleaned to allow the chamber interior to be viewed during testing.

4.7.3* Chamber Walls. The chamber walls shall be cleaned to prevent excessive build-up of smoke products.

4.7.4 Specimen Holders. Specimen holders and horizontal rods securing the holder position shall be cleaned by removing any charred residues to prevent contamination of subsequent specimens.

4.8 Ancillary Equipment.

4.8.1 Balance. The balance shall have a capacity exceeding the mass of the specimen and shall be readable and accurate to 0.5 percent of the specimen mass.

4.8.2 Timing Device. A timing device capable of recording elapsed time to the nearest second over a period of at least 1 hour, with an accuracy of 1 second in 1 hour, shall be used for timing operations and observations.

4.8.3 Linear Measuring Devices. Rules, calipers, gauges, or other devices shall be used for checking all dimensions specified with given tolerances.

4.8.4 Preheating of Chamber Heater. Preheating of the chamber to reach a stabilized temperature shall be permitted.

4.8.5 Protective Equipment. Protective clothing, such as gloves, goggles, and respirators, and handling equipment, such as tongs, shall always be available and shall be used when the type of sample being tested demands them.

4.8.6 Data Acquisition.

4.8.6.1 The recorder or data acquisition unit used shall be capable of continuously recording the millivolt output of the photodetector to an accuracy of better than 0.5 percent of full-range deflection as described in 4.5.3.

4.8.6.2 The device used shall also be capable of recording the heat flux meter output to the required accuracy as described in 4.3.4.2.

4.8.6.3 If a data acquisition unit is used, the data collection intervals shall be 5 seconds or less.

4.8.6.4 If a recorder is used, the recording chart drive shall be used at a minimum chart speed of 10 mm/min.

4.8.7* Thermometer. A thermometer or a Type K thermocouple shall be available and shall be capable of measuring temperature over the range 20°C to 100°C to an accuracy of $\pm 0.5^{\circ}\text{C}$.

4.8.8 Water Circulating Device. A device for water circulation shall be provided to cool the heat flux meter.

Chapter 5 Test Environment

5.1 Light Interference. The test apparatus shall be protected from direct sunlight or any strong light source, to avoid the possibility of spurious light readings.

5.2 Product of Combustion Venting.

5.2.1 Exhaust vents shall be provided for removing smoke and gases from the area of operation.

5.2.2 Precautions shall be taken to prevent exposure of the operator to such gases, particularly during the removal of specimens from the chamber or when the apparatus is being cleaned.

5.2.3 The exhaust system shall be checked for proper operation complying with 7.10.1 and Section 7.11 before testing.

5.3* Operator Safety.

5.3.1 The operator shall use heavy gloves, safety tongs, or other protection for removal of the specimen holder.

5.3.2 Care shall be taken not to touch the spark igniter.

5.3.3 Ejection of hot material or sharp fragments from some kinds of specimens when irradiated shall be taken into account.

Chapter 6 Test Specimen

6.1 Suitability of Sample for Testing.

6.1.1 Method.

6.1.1.1 The test method shall be intended for essentially flat samples only.

6.1.1.2 Essentially flat surfaces shall be those where the irregularity from a plane does not exceed ± 1 mm.

6.1.2 Sensitivity. The results of this test method shall be sensitive to variations in surface characteristics, thickness of individual layers, overall thickness, mass, and composition.

6.2 Sample Face. If the two faces of samples submitted for evaluation by this method are different, both faces shall be evaluated if it is possible that both faces will be exposed to fire when in use.

6.3* Number of Specimens.

6.3.1 A minimum of six specimens shall be tested, so that three specimens are tested at each of the two required conditions.

6.3.2 Unless otherwise specified by the test requester, the standard exposure conditions shall be as follows:

- (1) Flaming at an irradiance of 25 kW/m²
- (2) Flaming at an irradiance of 50 kW/m²

6.4 Additional Specimens.

6.4.1 An additional number of specimens, as specified in Section 6.3, shall be used for each face in accordance with the requirements of Section 6.2.

6.4.2 An additional six specimens (three specimens per mode to be tested) shall be held in reserve, in case they are required by the conditions specified in 9.9.2.

6.5 Size of Specimens.

6.5.1 Size. The specimens shall be square with sides 75 mm.

6.5.2 Thickness.

6.5.2.1 Whenever possible, test samples shall be in their end-use thickness.

6.5.2.2 Samples used with a thickness of 25 mm or less shall be evaluated at their full thickness.

6.5.2.3 If no information on sample thickness is available, materials shall be permitted to be tested at a thickness of 1.0 mm, unless otherwise specified in the material or performance standard or specification.

6.5.2.4 Samples with a thickness greater than 25 mm shall be cut to give a specimen thickness of 25 mm in such a way that the original (uncut) face is evaluated.

6.5.2.5 Samples of multilayer materials, products, or assemblies with a thickness greater than 25 mm, consisting of core material(s) with facings of different materials, shall be prepared according to 6.5.2.4 as described in Section 6.6.

6.6 Specimen Preparation.

▲ **6.6.1** The specimen shall be representative of the materials or composites and shall be prepared in accordance with the recommended application procedures.

■ **6.6.1.1** Flat sections of the same thickness and composition shall be tested rather than curved, molded, or specialty sections.

■ **6.6.1.2** Substrate or core materials for the test specimens shall be the same as those for the intended application.

■ **6.6.1.3** If a material or assembly has the potential to be exposed to a fire on either side, both sides shall be tested.

■ **6.6.1.4** If an adhesive is intended for field application on a finish material or substrate, the prescribed type of adhesive and the spreading rate recommended for the field application of the assembly of the test specimen shall be used and the details reported.

● **6.6.2** Paints, adhesives, or similar finish materials shall be applied to the smooth face of 6.4-mm thick uncoated fiber cement board, nominally 1440 ± 160 kg/m³ in density, in compliance with ASTM C1288, *Standard Specification for Fiber-Cement Interior Substrate Sheets*, or ASTM C1186, *Standard Specification for Flat Fiber-Cement Sheets*, Grade II, and using the recommended application techniques and coverage rates.

■ **6.6.3** Finish materials, including sheet laminates, tiles, fabrics, and other materials, secured to a substrate material with an adhesive shall be evaluated by performing supplementary tests on a split exposed surface.

■ **6.6.4** Composite materials not attached to a substrate, which have the potential to be subject to delamination, cracking, peeling, or other separations affecting their smoke generation, shall be evaluated by performing supplementary tests on an interior layer or surface.

■ **6.6.5** When supplementary tests, as required by 6.6.3 or 6.6.4, are conducted, the manner of performing such supplementary tests and the test results shall be included in the report with the results from the original tests.

■ **6.6.6** Finish materials without a substrate or core shall be tested using the procedures in 6.6.6.1 and 6.6.6.2.

■ **6.6.6.1** Rigid or semi-rigid finish materials, such as sheet materials or veneers, shall not require supplementary tests, regardless of thickness.

■ **6.6.6.2*** Veneers that are not rigid or semi-rigid materials and that are intended for application to combustible substrates shall be applied to the smooth face of 6.4-mm nominal tempered hardboard in compliance with ANSI/AHA A135.4, *Basic Hardboard*, and using the recommended application techniques and coverage rates unless a specified assembly system has been provided.

■ **6.6.6.2.1** Supplementary tests shall be conducted on the hardboard alone and the results shall be reported as supplemental to the measured values for the composite specimens.

■ **6.6.6.2.2** The results of the tests conducted with the backed veneers and those conducted with the hardboard alone shall be included in the test report.

■ **6.6.7** Fabrics and thin films that tend to shrink, bunch, blister, or pull out from under the specimen holder during the test shall be tested with the test specimens and the aluminum foil wrapper stapled to an inorganic insulation millboard backing and shall use five standard size wire staples, approximately 12.7 mm by 6.3 mm by 0.5 mm, centered horizontally at the center of the four quadrants.

N 6.6.8 Electrical or Optical Fiber Wires or Cables.

N 6.6.8.1 Electrical or optical fiber wires or cables up to 25.4 mm in diameter shall be tested by cutting the cables to 76.2 mm + 0 mm, -0.8 mm lengths.

N 6.6.8.2 Lengths of wire or cables prepared per 6.6.8.1 shall be placed side-by-side in the specimen holder until no additional lengths can be added.

N 6.6.8.3 A sheet of 12.7-mm thick inorganic insulation mill-board shall be wrapped with aluminum foil and placed behind the wires or cables as a backing board before the specimen holder spring and retaining rod are inserted.

6.7 Wrapping of Specimens.

6.7.1 All specimens shall be covered across the back, along the edges, and over the front surface periphery leaving a central exposed specimen area of 65 mm ± 5 mm × 65 mm ± 5 mm, with a single sheet of aluminum foil that is 0.04 mm ± 0.005 mm thick with the dull side in contact with the specimen.

6.7.1.1 Care shall be taken not to puncture the foil or to introduce unnecessary wrinkles during the wrapping operation.

6.7.1.2 The foil shall be folded so as to minimize losses of any molten material at the bottom of the holder.

6.7.1.3 After the specimen is mounted into its holder, any excess foil along the front edges shall be trimmed off.

6.7.2 All wrapped specimens shall be backed with one or more sheets of noncombustible insulating board of an oven-dry density of 850 kg/m³ ± 100 kg/m³ and a nominal thickness of 12.5 mm to ensure that the top edges of the specimen are pressed against the retaining lips of the specimen holder.

6.7.3 Wrapped specimens less than 25 mm thick shall be backed with at least one sheet of noncombustible board with or without a layer of refractory mineral fiber blanket underneath to accommodate a wider variety of specimen thicknesses as described in 4.3.5.2.

6.7.4 In the case of resilient materials, products, or assemblies, each specimen shall be installed in its aluminum foil wrapper in the holder in such a way that the exposed surface lies flush with the inside face of the opening of the specimen holder.

6.7.5 Specimens with uneven exposed surfaces shall not protrude beyond the plane of the opening of the specimen holder.

6.7.6 When thin impermeable specimens, such as thermoplastic films, swell during the test due to gases trapped between the film and the backing, the specimens shall be maintained essentially flat by making two or three cuts 20 mm to 40 mm long in the film to act as vents.

Chapter 7 Setup, Calibration, and Maintenance

7.1* Setup and Calibration Procedures. The test apparatus shall be assembled, connected to the services and control devices as specified in Chapter 8, and checked for compliance with the procedures as noted in Section 7.2 through Section 7.11 and for the operation of the various systems, including the electrical connections.

7.2 Alignment of Photometric System.

7.2.1 General.

7.2.1.1 The setup procedure shall be conducted as detailed in 7.2.2 and 7.2.3 in the initial setup of the apparatus, after the replacement of the light source or after the occurrence of some accidental misalignment.

7.2.1.2 The procedure for selecting the compensating filter(s) shall be followed after each setup procedure as described in Section 7.3.

7.2.2 Beam Collimation.

7.2.2.1 The optical platforms shall be checked for rigidity.

7.2.2.1.1 The opaque-disc template shall be attached to the lower face of the upper optical window with the marked ring downward and centered on the window.

7.2.2.1.2 The light source shall be switched on and its projected image adjusted on the template, so that the light beam completely fills the 51 mm diameter ring with no more light outside the ring than is necessary to satisfy this requirement.

7.2.2.2* Adjustments shall be made by removing the cover to the light source enclosure, releasing the lower lens mount fixings, and repositioning the lens mount, so that the light pattern on the template is centered and of the correct size.

7.2.2.3* The lens mount shall be reaffixed and the cover replaced, ensuring that the test cabinet has been resealed.

7.2.2.4 The template shall be removed from the upper optical window.

7.2.3 Beam Focusing.

7.2.3.1 The cover to the housing on top of the test chamber shall be opened, the compensating filter holder shall be removed, and the lens mount shall be slackened.

7.2.3.2 With the photodetector system switched off and the light source switched on, the lens mount shall be adjusted for focusing and alignment, so that the converging beam forms a small intense spot of light on the aperture to the photomultiplier tube housing.

7.2.3.3 The lens mount shall be tightened, the beam focusing adjustment shall be checked, the compensating filter holder shall be replaced, and the enclosure cover shall be closed and sealed.

7.3* Selection of Compensating Filter(s).

7.3.1 The faces of both optical windows inside the test chamber shall be cleaned.

7.3.2 The photometric system shall be switched on with the range-extension filter in the light path, the shutter open (if applicable), and the multirange meter set to the range capable of recording 100 percent light transmission.

7.3.3 The control for adjusting the reading of the instrument shall be operated to determine whether 100 percent light transmission is achievable. If 100 percent is achievable, no change in the compensating filter shall be required; if 100 percent is not achievable, another compensating filter shall be used to satisfy this requirement.

7.4 Linearity Check.

7.4.1 The photometric system shall be switched on with the range-extension filter in the light path and the shutter closed.

7.4.1.1 The zeroing device shall be adjusted, with the instrument range switched to the most sensitive range, to give a reading of 0 percent light transmission with the instrument range switched to a full-scale reading of 100 percent transmission.

7.4.1.2 The instrument shall be switched to the other ranges to determine that the recorded transmission remains 0 percent.

7.4.2 The calibrated filter having a nominal optical density of 3.0 shall be placed in the light path over the lower optical window, the shutter shall be opened, and the percentage of transmission shall be measured.

7.4.3 The difference between the observed reading and the calibrated value, when expressed as a percentage of the average of the two values, shall be within 5 percent.

7.5 Calibration of Range-Extension Filter.

7.5.1 The test apparatus shall be brought to an incident heating flux of 25 kW/m² as described in Section 9.1 with the chamber wall temperature remaining steady at 40°C ± 5°C.

7.5.2 The photometric system with the range-extension filter in the light path and with the shutter open shall be switched on, and the amplifier shall be switched to its 100 percent transmission range.

7.5.3 The white cloth, sheets of tissue, or filter with an optical density of about 2.5 shall be placed over the lower optical window and the amplifier switched to the 1 percent transmission range as described in 4.5.3.

7.5.4 The reading shall be set to 0.50 percent by adjusting the instrument.

7.5.5 Without disturbing the cloth, tissue, or filter, the amplifier shall be reset to the 100 percent transmission, and the ND-2 range-extension filter shall be withdrawn from the light path.

7.5.6 The transmission reading, T_p , shall be recorded and used to determine the value of the correction factor, C_p , from Table 7.5.6 for readings obtained when the range-extension filter is not in the light path.

7.5.7 For materials, products, or assemblies having known performance, the calibration procedure in 7.5.1 through 7.5.6 shall not be needed unless the optical density is greater than 3.

7.6 Chamber Leakage Rate Test.

7.6.1 The airtightness of the test chamber shall be measured on each occasion of use (with the door, vents, and spare gas sampling pipes closed) by introducing compressed air into the test chamber through one of the gas sampling pipes (or other compressed air inlet) until the pressure recorded on the manometer is over 0.76 kPa and then shutting off the supply.

7.6.2 The airtightness of the test chamber shall be such that the time taken for the recorded pressure to drop from 0.76 kPa to 0.50 kPa, as determined by using the timing device, shall be not less than 5.0 minutes.

Table 7.5.6 Correction Factors with Neutral Density Filter (ND-2) Removed

Meter Indication (T_p)	Correction Factor (C_p)	Optical Density of Neutral Density Filter
31	-27.4	1.79
32	-25.6	1.81
33	-23.8	1.82
34	-22.1	1.83
35	-20.4	1.845
36	-18.8	1.86
37	-17.3	1.87
38	-15.7	1.88
39	-14.2	1.89
40	-12.8	1.90
41	-11.4	1.91
42	-10.0	1.92
43	-8.6	1.93
44	-7.3	1.94
45	-6.0	1.95
46	-4.8	1.96
47	-3.5	1.97
48	-2.3	1.98
49	-1.2	1.99
50	0.0	2.00
51	+1.1	2.01
52	+2.2	2.02
53	+3.3	2.025
54	+4.4	2.03
55	+5.5	2.04
56	+6.5	2.05
57	+7.5	2.06
58	+8.5	2.064
59	+9.5	2.07
60	+10.5	2.08
61	+11.4	2.086
62	+12.3	2.09
63	+13.2	2.10
64	+14.2	2.107
65	+15.0	2.114
66	+15.9	2.12
67	+16.8	2.13
68	+17.6	2.135
69	+18.5	2.14
70	+19.3	2.146

7.7* Burner Calibration. The propane and air flows shall be set to obtain the flame dimensions, color, and positioning required in 4.3.6 as described in Section 4.4.

7.8 Radiator Cone Calibration.

7.8.1 Cleaning. The test apparatus shall be cleaned of any residues left from previous tests.

7.8.1.1 When a cone calibration is to follow soon after a test, the chamber shall be flushed with air for 2 minutes, with the door shut and the exhaust and inlet vents open.

7.8.1.2 The heat flux meter shall be mounted as specified in 4.3.2.1 and shall be connected to the electrical and water services.

7.8.2 Burner Ignition. The burner shall not be ignited during this calibration.

7.8.3 Temperature. The test apparatus shall be brought to its normal operating condition as described in Section 9.1, with the chamber wall temperature remaining steady as described in 9.1.3.3 and the radiator shield moved away from the radiator cone.

7.8.4* Water Supply. With the chamber door closed, the inlet vent open, and the exhaust vent closed, water shall be supplied to the heat flux meter to cool the heat flux meter body.

7.8.4.1 The heat flux meter output shall be monitored to determine when thermal equilibrium has been reached.

7.8.4.2 The cone shall then be adjusted, as necessary, to give a steady millivolt reading corresponding to the calibrated value equivalent to an irradiance of 25 kW/m² or 50 kW/m², as required.

7.8.4.3 If the door is opened for any reason during calibration, at least 10 minutes shall be allowed after closing the door for thermal equilibrium to be reached before taking the final millivolt reading.

7.8.5 Repeat Procedure. The procedure in 7.8.4 shall be repeated as necessary to calibrate the equipment in three positions — at the center and at 25 mm ± 1 mm on each side of the center.

7.8.6 Radiator Shield.

7.8.6.1 The radiator shield shall be returned to the position below the cone, and the heat flux meter shall be removed from the test chamber so that tests on specimens can proceed immediately.

7.8.6.2 Water shall be circulated through the heat flux meter until the meter is cool enough for the protective cap to be replaced without melting or distortion.

7.9* Cleaning. The inside walls of the test chamber and the supporting framework for the cone and specimen holders shall be cleaned using materials as described in Section 4.7, whenever periodic visual inspection indicates the need.

7.10 Frequency of Checking and Calibrating Procedures.

7.10.1* Regular checking and calibration shall be undertaken in accordance with Table 7.10.1.

7.10.2 The relevant setup procedure shall be followed after any part of the equipment has been renewed or repaired.

Table 7.10.1 Frequency of Checks and Calibrations

Item of Equipment	Maximum Interval Between Checks and Calibrations	Procedure (Section Reference)
Test chamber interior	Before testing every specimen and before any calibration	7.9
Radiator cone	Once every test day and when renewed or replaced	7.8
Chamber leakage rate	Once every test day and when new seals or safety blow-out panel are fitted	7.6
Heat flux meter	Every 3 months and when cleaned or recoated	4.3.4.3
Photometric system:		
Calibration	Before testing every specimen	9.3
Alignment	Every 6 months and when light source is replaced or when damage is incurred	7.2
Compensating filters	Every 6 months and when transmission through windows deteriorates	7.3
Linearity	Every 6 months and when transmission through windows deteriorates	7.4
Range-extension filter	Every 6 months	7.5
Total system	Every month or after the system has been used for more than 100 tests	7.11

7.11* Total System.

7.11.1 The total system shall be checked by testing a material or product with repeatable results.

7.11.2 A record of the test results shall be maintained; if erratic values are observed, any instrumental or operational deficiencies shall be identified and corrected.

Chapter 8 Conditioning

8.1 Pre-Test.

8.1.1 Prior to testing, the specimens shall be conditioned to constant mass in an atmosphere at a temperature of $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$ and a relative humidity of 50 percent ± 10 percent.

8.1.2 Constant mass shall be considered to have been reached when two successive weighing operations carried out at an interval of 24 hours do not differ by more than 0.1 percent of the mass of the test piece or 0.1 g, whichever is greater.

8.1.3 The specimen shall be tested within 10 minutes of removal from the conditioning atmosphere if the test room conditions differ from the above.

8.2* Conditioning. While in the conditioning chamber, specimens shall be supported in racks so that air has access to all surfaces.

Chapter 9 Test Procedure

9.1 Initial Conditions.

9.1.1 The mass of each test specimen wrapped in aluminum foil shall be recorded before placing it inside the specimen holder, to generate an initial mass, m_i (in grams).

9.1.2 The test chamber shall be prepared according to the requirements of Chapter 7, with the radiator cone set at an irradiance of 25 kW/m^2 or 50 kW/m^2 .

9.1.3* If a test has just been completed, the test chamber shall be flushed with air with the test chamber door closed and the exhaust and inlet vents open, until it is completely clear of smoke.

9.1.3.1 The inside of the cabinet shall be inspected and the walls and the supporting framework shall be cleaned whenever necessary, as described in Section 7.9.

9.1.3.2 The faces of the optical windows inside the chamber shall be cleaned before each test.

9.1.3.3 The apparatus shall be allowed to stabilize until the chamber wall temperature is within the range of $40^{\circ}\text{C} \pm 5^{\circ}\text{C}$ for tests with the radiator cone at 25 kW/m^2 or within the range $55^{\circ}\text{C} \pm 5^{\circ}\text{C}$ for tests with the radiator cone at 50 kW/m^2 .

9.1.3.4 The inlet valve shall be closed.

9.2 Tests with Pilot Flame.

9.2.1 For tests with the pilot flame, with the burner in its correct position, the gas and air supplies shall be turned on, and the burner shall be ignited.

9.2.1.1 The flow rates shall be checked.

9.2.1.2 If necessary, the flow rates shall be adjusted to ensure that they are in accordance with Section 7.7.

9.2.2 If the pilot flame is extinguished by gaseous effluent during a test and fails to reignite within 10 seconds, the gas supply to the pilot burner shall be switched off immediately.

9.3 Preparation of Photometric System. The photometric system shall be prepared as follows:

- (1) Set the recorder to zero and then open the shutter to set the full-scale 100 percent transmission reading.
- (2) Close the shutters and check and reset the recorder to zero, if necessary, using the most sensitive 0.1 percent range.
- (3) Recheck the 100 percent setting.
- (4) Repeat the sequence of operations until 100 percent accurate and zero readings are obtained on the amplifier and recorder or on the data acquisition unit when the shutters are opened and closed.

9.4 Loading Specimen.

9.4.1 A wrapped specimen prepared in accordance with Sections 6.3 and 6.4 with its insulating board as noted in 6.7.2 shall be placed in its holder.

9.4.1.1 The specimen holder and specimen shall be placed on the supporting framework below the radiator cone.

9.4.1.2 The test chamber door shall be closed immediately.

9.4.2 The test shall be started by removing the radiator shield from below the cone and simultaneously starting the recording chart drive or data acquisition unit and closing the inlet vent.

9.4.3 If preliminary tests indicate that the pilot flame is extinguished before the radiator shield is removed, this problem with the equipment shall be remedied before continuing with the test.

9.5 Recording of Light Transmission.

9.5.1 The percentage of light transmission and the corresponding time shall be recorded continuously from the start of the test, that is, from the time the radiator shield is removed.

9.5.2 The range of the photodetector amplifier system shall be switched to the next decade when required so that readings less than 10 percent of full-scale deflection are avoided.

9.5.3 If the light transmission falls below 0.01 percent, the observation window in the chamber door shall be covered and the range-extension filter shall be withdrawn from the light path.

9.5.4 The range shall be switched to a full scale of 1 percent to give an effective full-scale range of 0.01 percent.

9.6* Observations. Any particular burning characteristics of the specimens, such as delamination, intumescence, shrinkage, melting, dripping, collapse, or occurrence of pool fire under the test specimen, or any other event of special interest shall be recorded, and the time at which the particular behavior occurs, including the time to ignition and duration of flaming, also shall be recorded.

9.6.1 The smoke characteristics, such as color and the nature of the settled particulate matter, shall be recorded.

9.6.2 All times shall be reported from the moment the test was started as described in 9.4.2.

9.7 Termination of Test.

9.7.1 The test shall be conducted for a period of 10 minutes.

9.7.1.1 The test shall be permitted to be conducted for periods in excess of 10 minutes when minimum light transmittance values have not been reached during a 10-minute exposure.

9.7.1.2 If the period exceeds 10 minutes, the test time shall be reported.

9.7.2* The burner shall be extinguished if the pilot flame has been used.

9.7.3 The radiator shield shall be moved below the cone.

9.7.4 The exhaust fan shall be switched on, and when the manometer indicates a small negative pressure, the inlet vent shall be opened and shall continue exhausting until a maximum value of light transmission is recorded, with the most sensitive range selected, and noted as the “clear beam” reading, T_c for use in correcting for deposits on the optical windows.

9.8 Specimen Mass.

9.8.1 At the conclusion of each test, the final specimen mass, m_f (in grams), shall be determined after the specimen is removed from the specimen holder.

9.8.2 The aluminum foil in which the specimen was wrapped during the test for determining the mass shall be included.

9.9 Repeat Tests.

9.9.1 The percentage of light transmission of two sets of three specimens for each sample, one set for each mode from among the four standard exposure conditions shown in 9.2.2, shall be measured.

9.9.2 The following default exposure conditions, unless specified otherwise by the test requester, shall be those with a pilot flame:

- (1) Mode 1: Irradiance — 25 kW/m² with pilot flame
- (2) Mode 2: Irradiance — 50 kW/m² with pilot flame
- (3) Mode 3: Irradiance — 25 kW/m² without pilot flame
- (4) Mode 4: Irradiance — 50 kW/m² without pilot flame

9.9.3 If during a test one or more of the three replicate specimens show any of the following behaviors, an additional specimen of the identical preconditioned sample shall be tested in the test mode in which the unusual behavior(s) occurred:

- (1) Self-ignition of a specimen occurs in the nonflaming mode.
- (2)* A specimen is displaced from the zone of controlled irradiance so as to touch the pilot burner or the pilot flame.
- (3) The pilot flame is extinguished (even for a short period of time) in the flaming mode. The test results of a specimen that does not cease flaming after the pilot flame goes out shall not be considered valid, and additional tests shall not be required.
- (4) Molten material overflows the specimen holder.

9.9.4 A maximum of six specimens shall be allowed to be tested.

9.9.5 Data obtained from the improper tests noted in 9.9.3(1) through 9.9.3(4) shall not be incorporated in the averaged data, but the occurrence shall be reported.

9.9.6 The test method shall not be suitable if three or more of the specimens tested show any of the characteristics in 9.9.3(1) through 9.9.3(4).

9.9.7 For each individual specimen, the percentage value of light transmission shall be determined, and the specific optical density from this value shall be calculated, as given in Chapter 10.

9.9.8 If the specific optical density value (D_s) at 10 minutes for an individual specimen differs by more than 50 percent from the average for the set of three specimens of which it is part, an additional set of three specimens shall be tested from the same sample in the same mode, and the average of all six results obtained shall be recorded.

Chapter 10 Calculations

10.1 Specific Optical Density, D_s .

10.1.1 For each specimen, the set of continuous recorded data of light transmission against time shall be used, and the results at 1.5 minutes, 4.0 minutes, and 10.0 minutes shall be converted to specific optical density, D_s , by using the following equation, where $T\%$ is a value of the percent light transmittance, taken from the continuous record:

[10.1.1]

$$D_s = 132 \log_{10} \frac{100}{T\%}$$

10.1.2 The factor 132 shall be derived from the physical characteristics of the chamber by using the following equation:

[10.1.2]

$$\frac{V}{A \times L} = 132$$

where:

V = volume of the chamber

A = exposed area of the specimen

L = length of the light path

10.1.3 A correction factor, C_p , shall be added to the value of D_s , as determined in 10.1.1.

10.1.3.1 This correction factor shall depend upon the use of the range-extension filter.

10.1.3.2 The value of C_p shall be zero if one of the following applies:

- (1) The filter is in the light path at the time the transmission was recorded ($T\% \geq 0.01\%$).
- (2) The photometric system is not equipped with a removable filter.
- (3) The ND-2 filter is of the correct optical density of 2.

10.1.3.3 The value of C_f shall be as determined by the procedure described in Section 7.5 and Table 7.5.6 if the filter is moved out of the light path at the time it is measured ($T\% < 0.01\%$).

10.2 Clear Beam Correction Factor, D_c

10.2.1 For each specimen, the value of the “clear beam” reading, T_c , shall be recorded to determine the correction factor D_c as described in 9.7.4.

10.2.2 D_c shall be calculated as for D_s in Section 10.1.

10.2.3 The correction factor D_c shall not be required to be recorded if it is less than 5 percent of the maximum specific optical density as determined from that created by plotting the recording of light versus time in Section 10.1 and 11.2(3) as described in Section 10.1.

10.3* Mass Loss. For each valid specimen tested, the total mass loss, D_m (in grams), shall be calculated and recorded using the following equation:

[10.3]

$$D_m = m_1 - m_2$$

where:

m_1 = initial mass of the specimen (including the aluminum foil used for testing) (g)

m_2 = mass of the specimen after the test (with all the foil wrappings included) (g)

Chapter 11 Test Report

11.1 Descriptive Information. The following descriptive information shall be included in the test report:

- (1) Name and address of the testing laboratory
- (2) Date and identification number of the report
- (3) Name and address of the test requester, when applicable
- (4) Name of the manufacturer or supplier of material, product, or assembly tested, if known
- (5) Commercial name or other identification marks and description of the sample
- (6) Full description of the sample, including such details as type, form, essential dimension, mass or density, color, and coverage rate of any coating
- (7) Full description of specimen construction and preparation as described in Sections 6.5 and 6.6
- (8) Face of specimen tested as described in Sections 6.5 and 6.6
- (9) Thickness of each specimen tested
- (10) Conditioning of the test specimens
- (11) Date of the test
- (12) Modes of testing, indicating irradiance and use of the pilot flame for each specimen
- (13) Number of specimens tested for each type of exposure
- (14) Test number and any special remarks

▲ 11.2 Test Results. The following test results shall be included in the test report:

- (1) A table of numerical results containing the following information for each valid specimen tested:
 - (a) Specific optical density at 1.5 minutes
 - (b) Specific optical density at 4.0 minutes
 - (c) Specific optical density at 10.0 minutes
 - (d) Specific optical density at end of the test (if test duration is longer than 10.0 minutes)
 - (e) Maximum specific optical density
 - (f) Time to ignition
 - (g) Time to maximum optical density
 - (h) Duration of the test
 - (i) If calculated, the neutral density correction, C_f
 - (j) The clear beam correction factor, D_c
 - (k) The mass loss, D_m
- (2) Graphical results for each valid specimen tested
- (3) Graph of specific optical density against time
- (4) All the available information required in Section 6.7 (regarding specimen preparation and coatings used, if applicable) and Section 9.6 (observations regarding burning characteristics of the specimens and any events of special interest during the tests)
- (5) Details of any invalid tests, including the reasons for them being invalid as described in 1.3.3.1 and 9.9.3
- (6) Details of any supplementary tests conducted, including information on the supplementary test itself and the test results

Annex A Explanatory Material

Annex A is not a part of the requirements of this NFPA document but is included for informational purposes only. This annex contains explanatory material, numbered to correspond with the applicable text paragraphs.

A.1.1.2 This test method is technically equivalent to ISO 5659-2, *Plastics — Smoke generation — Part 2: Determination of optical density by a single-chamber test*, and to ASTM E1995, *Standard Test Method for Measurement of Smoke Obscuration Using a Conical Radiant Source in a Single Closed Chamber, With the Test Specimen Oriented Horizontally*.

A.1.1.7 For limitations of this test method, see 1.3.3.

A.1.1.9 This test method is known to involve hazardous materials, operations, and equipment as described in 5.2.2, 5.2.3, and 9.7.2.

A.1.3.1.6 See Annex D for additional information on mass optical density.

A.1.3.2.1 The current smoke density chamber test, ASTM E662, *Standard Test Method for Specific Optical Density of Smoke Generated by Solid Materials*, is used in the United States by specifiers of floor coverings and in the rail transportation industry. The measurement of smoke obscuration is important to the researcher and the product development scientist. This test method also increases the usefulness of smoke obscuration measurements to specifiers and to product manufacturers.

A.1.3.2.2 The photometric scale used to measure smoke by this test method is similar to the optical density scale for human vision. As with many smoke obscuration test methods, correlation with measurements by other test methods has not been established.

A.1.3.2.3 No basis exists for predicting the smoke obscuration by specimens not exposed to the specified fire conditions.

A.1.3.3.2 Results obtained from this test method have proven to be affected by small variations in sample geometry, surface orientation, thickness (either overall or individual layer), mass, and composition. Therefore, it is critical that the replicate

samples be cut, sawed, or blanked to identical sample areas, and that records be kept of the respective masses with the individual test data.

Preselection of samples with identical thickness or mass, or both, will reduce the variation but is not necessarily indicative of the actual variation to be expected from the sample as normally supplied.

A.1.3.3.3 There is no simple mathematical formula applicable to calculate the specific optical density of thickness of a sample different from the sample tested. Some information on a relationship between optical density and thickness is found in Grand, "Defining the Smoke Density Hazard of Plastics."

Results obtained from this test method are affected by small variations in the position of the sample and radiometer relative to the radiant heat source.

A.1.3.3.4 Even when the same sample is being tested, excessive accumulations of residue should not be permitted to build up, since ruggedness tests have indicated that such deposits serve as additional insulators, tending to reduce normally expected condensation of the aerosol, thereby raising the measured specific optical density.

A.1.3.3.5 The measurements obtained have also proven sensitive to small differences in conditioning (see Chapters 7 and 8). Many materials, products, and assemblies, such as carpeting and thick sections of wood, plastics, or plywood, require long periods to attain equilibrium (constant weight) even in a forced-draft conditioning chamber.

This test method solves some of the limitations associated with other closed-chamber test methods, such as ASTM E662, *Standard Test Method for Specific Optical Density of Smoke Generated by Solid Materials*, but some additional limitations remain.

A.1.3.3.6 The atmosphere inside the chamber during some tests becomes oxygen deficient before the end of the experiment, and combustion often ceases when the oxygen concentration decreases. Therefore, for heavy composites, for example, it is possible that the layers farthest away from the radiant source will not undergo combustion. Walls cause losses of combustion particulates through deposition. (See Annex D for additional information.)

A.1.3.3.7 Soot and other solid or liquid combustion products settle on the optical surfaces during a test, resulting in potentially higher smoke density measurements than those caused by the smoke in suspension.

A.4.2.2 Stainless steel wire mesh offers adequate protection for the blow-out panel.

A.4.2.3.2 The internal heater should be able to heat the chamber to a temperature just sufficient to minimize smoke condensation on that face. A temperature of 50°C to 55°C has been found suitable for that purpose.

A.4.2.6 A suitable pressure regulator should consist of an open water-filled bottle and a length of flexible tubing inserted 100 mm below the water surface; the other end of the tubing should be connected to the manometer and the chamber. (See Figure A.4.2.6.) The regulator should be vented to the exhaust system.

A.4.3.1.3 It has been found that thermocouples of equal length and wired in parallel to the temperature controller

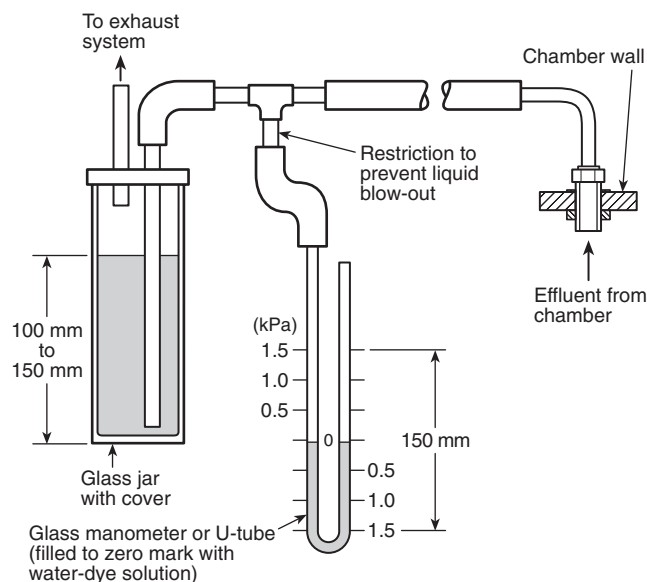


FIGURE A.4.2.6 Typical Chamber Pressure Relief Manometer.

perform adequately; alternative wiring methods shown to give equivalent results are also acceptable. Sheathed Chromel®/Alumel® Type K thermocouples have been found suitable for this purpose.

A.4.3.1.4 An irradiance of 50 kW/m² will be given by a heater temperature in the 700°C to 750°C temperature range.

While phase-angle control is allowed for the temperature controller of the radiator cone, it should be noted that this control will usually require electrical filtering to avoid the risk of inducing noise in lines with low signal levels.

A.4.3.3.2 The radiator shield handle is necessary to enable repeat tests to be carried out without switching off the radiator cone.

A.4.3.4.1 The manufacturer of Schmidt-Boelter gauges has the following specifications for cooling water: pressure 413,621 kPa, temperature 20.0°C to 26.6°C, and flow rate 0.76 L/min to 1.14 L/min.

A.4.3.4.2 If a recorder that displays only a millivolt output is used, the millivolt value should be converted to heat flux, in kilowatts per square meter, using the calibration factor (or equation, if appropriate) specific to the heat flux meter.

A.4.3.5.3.1 The retainer frame and wire grid are particularly appropriate when testing intumescent specimens and also for reducing unrepresentative edge combustion of composite samples or for retaining specimens prone to delamination. The wire grid is likely to affect the test results, compared with tests conducted in its absence. However, its use is recommended for several reasons: it helps to promote uniformity in testing by different laboratories; in view of the expected effect of the retainer frame and wire grid on test results as explained above, it is needed for certain specimens; and it is required in ISO 5659-2, *Plastics — Smoke generation — Part 2: Determination of optical density by a single-chamber test*.

A.4.3.6 It is recommended that a small-spark ignition device be sited next to the outlet tube of the burner, allowing the operator to ignite the flame without opening the door of the chamber. A suitable system is a spark plug with a 3 mm gap powered from a 10 kV transformer. A suitable transformer is of a type specifically designed for spark ignition use, with an isolated (ungrounded) secondary to minimize interference with the data transmission lines. An acceptable electrode length and spark plug location is such that the spark gap is located 13 mm above the specimen, close to the pilot burner.

A.4.5.3.1 The required accuracy of the photodetector is obtained more easily if the measuring systems incorporate scale ranges of 30, 3, 0.3, and so forth, as well as ranges of 100, 10, 1, and so forth.

A.4.5.3.4 All filters should be handled by their edges because fingerprints greatly affect their rating. The surface of a filter should not be cleaned; once the surface has been damaged, the filter should be replaced.

A.4.6 The chamber should be sufficiently airtight to prevent smoke leakage. The most likely sources of leakage have been found to be the door seal, the inlet and outlet vents, and the safety blow-out panel.

A.4.7 Periodic cleaning is essential for proper operation. Appropriate materials for cleaning the inside of the chamber should be made available.

A.4.7.1 Clean the top window first, then the bottom window, using a nonabrasive cloth dampened with a suitable cleaner. Ethyl alcohol, ethyl ketone, or the equivalent, and soft tissue have been found effective for cleaning the optical windows and the viewing window. Dry the window to prevent streaking or film buildup. Do not use any cleaners that contain wax because wax will cause the smoke to be adsorbed to the glass more quickly.

A.4.7.3 An ammoniated spray detergent and soft scouring pads have been found effective for cleaning the chamber walls.

A.4.8.7 The thermometer is intended for determining ambient temperature or any other needed temperature.

A.5.3 The test procedure involves high temperatures and combustion processes. Therefore, it is possible for eye injuries, burns, ignition of extraneous objects, and inhalation of smoke or combustion products to occur unless proper precautions are taken. To avoid accidental leakage of toxic combustion products into the surrounding atmosphere, it is advisable to evacuate the chamber at the end of a test into an exhaust system with adequate capacity.

A.6.3 Optional testing modes include the following:

- (1) Nonflaming at an irradiance of 25 kW/m² (for comparison with the test results from ASTM E662, *Standard Test Method for Specific Optical Density of Smoke Generated by Solid Materials*)
- (2) Nonflaming at an irradiance of 50 kW/m² (for comparison with the test results from ISO 5659-2, *Plastics — Smoke generation — Part 2: Determination of optical density by a single-chamber test*)

These exposures are not required. Other testing modes are also possible with this equipment.

N A.6.6.6.2 Tempered hardboard sheets conforming to ANSI/AHA A135.4, *Basic Hardboard*, are marked with a 12.7-mm wide single red stripe placed on the thickness side approximately 76 mm from each corner. Service-tempered hardboard sheets are marked with two red stripes.

A.7.1 The radiator cone should be heated gradually from cold and not allowed to overheat or to remain operating without a blank specimen holder; that is, the holder should have a specimen in it or the heat flux meter in position in front of it.

A.7.2.2.2 In cases of severe maladjustment, the lamp socket should be repositioned also.

A.7.2.2.3 On occasion, this adjustment also includes the optimization of the lens mount position, so that the photodetector gives a maximum reading. This operation will require removal of the template and should be followed by a final check on the position of the image as described in 7.2.2.2.

A.7.3 An indication of the appropriate filter or combination of filters is obtained conveniently by removing any compensating filter(s) in the housing above the test chamber, closing the housing cover, placing a compensating filter(s) over the lower optical window inside the test chamber, and checking the instrument reading. The choice of compensating filter(s) determined this way needs to be confirmed by the specified procedure.

A.7.7 Typical flows required to obtain the correct flame are a propane flow of 88.5 cm³/min ± 1.0 cm³/min and an airflow of 270 cm³/min ± 20 cm³/min.

A.7.8.4 It is necessary for some water circulators to have the chamber door slightly open to allow access for the tubing. Allow at least 10 minutes for stabilizing between adjustments.

A.7.9 Because the test is sensitive to variations in the composition of samples, the apparatus should be cleaned when changing from tests on one material, product, or assembly to another so that the results are not affected by chemical or physical interaction between the specimen and the residues left from previous tests on products. Even when testing specimens of the same material, product, or assembly, accumulations of residue reduce the amount of deposition of smoke, resulting in an increase in the measured value of specific optical density.

A.7.10.1 Products of combustion of some materials, products, or assemblies might cause corrosion of the cone heating element. This corrosion can be compensated for by adjusting the applied voltage for a limited amount of change. If the cone cannot be made to give the required output, a new heating element might be required.

A.7.11 The material should be one that is, and is likely to continue to be, consistently available to the testing laboratory.

A.8.2 Forced-air movement in the conditioning chamber is acceptable to assist in accelerating the conditioning process. The results obtained from this method are sensitive to small differences in specimen conditioning. It is important, therefore, to ensure that the requirements of Sections 8.1 and 8.2 are followed carefully.

A.9.1.3 If the temperature is too high, use of the exhaust fan to draw in cooler air from the laboratory is an adequate procedure.

A.9.6 Smoke generation from some materials, products, or assemblies differs significantly depending on whether combustion occurs in a nonflaming or a flaming mode. It is important, therefore, to record as much information as possible about the mode of combustion (e.g., the presence of flame on the specimen surface) during each test.

Coated and faced samples, including sheet laminates, tiles, fabrics, and other composites secured to a substrate with an adhesive, and composites not attached to a substrate are subject to delamination, cracking, peeling, or other separations affecting their smoke generation.

A.9.7.2 The burner is extinguished in order to reduce the likelihood that the air added during venting will create an explosive mixture in the chamber.

A.9.9.3(2) If a thin specimen that had not been cut (*see* 6.7.6) swells out of the plane, the results from that specimen should be ignored and an extra cut specimen tested.

A.10.3 Note that the deposition of smoke particulates on walls and lens is one of the reasons that if two materials reach the same peak optical density at different times within the test, they are likely to exhibit different fire performance in terms of smoke obscuration and possibly in terms of mass optical density.

Annex B Precision and Bias

This annex is not a part of the requirements of this NFPA document but is included for informational purposes only.

B.1 Precision. Table B.1(a) and Table B.1(b) contain information on repeatability and reproducibility, based on a preliminary international interlaboratory evaluation in which batches of 16 materials were tested in accordance with this test method by eight laboratories in six countries, for plastic materials [Table B.1(a)] and building materials [Table B.1(b)]. Additional information on repeatability on two wood samples in a single laboratory is presented in Table B.1(c), and repeatability information from another laboratory, which tested six building products, is shown in Table B.1(d). Overall, the results of these preliminary studies indicate that the average coefficient of variation (CV%) for repeatability is 14.4, while the average coefficient of variation for reproducibility in the international study is 49.0. Results from a more definitive precision study will be made available after a round-robin evaluation has been completed.

B.2 Bias. The bias of this test method is unknown.

Table B.1(a) Repeatabilities and Reproducibilities of Specific Optical Density for Some Plastics

Material	Thickness (mm)	Irradiance (kW/m ²)	Mean, D_s (10 min)	Repeatability (Within Laboratories)		Reproducibility (Between Laboratories)	
				r	Percent of Mean	R	Percent of Mean
PMMA	1.0	25	11	4	38	10	91
		25 + pf	55	13	24	29	53
		50	54	11	20	17	32
ABS	1.1	25	312	77	25	311	100
		25 + pf	441	146	33	205	46
		50	435	102	23	192	44
Polyurethane rigid foam (28 kg/m ³)	25.0	25	49	16	32	61	124
		25 + pf	48	24	51	26	54
		50	145	48	33	97	67
Polyurethane flexible foam (27 kg/m ³)	25.0	25	178	49	27	114	64
		25 + pf	80	28	35	56	70
		50	127	46	36	80	63
Expanded polystyrene (nonfire retardant; 14 kg/m ³)	25.0	25	112	75	67	196	175
		25 + pf	102	75	74	130	128
		50	270	88	33	195	72

Note: "pf" indicates test carried out with pilot flame.

Table B.1(b) Repeatabilities and Reproducibilities of Specific Optical Density for Some Building Materials

Material	Thickness (mm)	Irradiance (kW/m ²)	Mean, D_s (10 min)	Repeatability (Within Laboratories)		Reproducibility (Between Laboratories)	
				r	Percent of Mean	R	Percent of Mean
Pine	12.1	25	403	97	24	300	74
		25 + pf	26	15	55	56	322
		50	196	191	98	191	98
Chipboard	12.2	25	411	47	12	187	45
		25 + pf	58	59	102	88	153
		50	481	96	20	464	97
Plywood	4.2	25	251	31	12	132	52
		25 + pf	33	15	47	58	175
		50	113	58	31	82	72
Medium density fiberboard	11.9	25	420	127	30	281	67
		25 + pf	68	42	62	72	106
		50	688	114	17	413	60
Paper-faced plasterboard	12.7	25	20	8	42	21	107
		25 + pf	8	8	104	25	314
		50	17	11	64	23	132

Note: “pf” indicates test carried out with pilot flame.

Table B.1(c) Repeatability Experiments Using Wood Samples in a Single Laboratory

Material	Douglas Fir Plywood	Red Oak Flooring
Incident flux: 25 kW/m ² , NF		
D_m (AVG)	496	475
D_m (STD)	47	9
D_m (CV%)	9	2
D_m /g (mass loss) (AVG)	24.2	22.1
D_m /g (mass loss) (STD)	4.7	7.3
D_m /g (mass loss) (CV%)	20	33
Incident flux: 35 kW/m ² , NF		
D_m (AVG)	475	461
D_m (STD)	11	12
D_m (CV%)	2	3
D_m /g (mass loss) (AVG)	19.9	11.9
D_m /g (mass loss) (STD)	3.4	2.7
D_m /g (mass loss) (CV%)	17	23
Incident flux: 40 kW/m ² , NF		
D_m (AVG)	491	461
D_m (STD)	13	22
D_m (CV%)	3	5
D_m /g (mass loss) (AVG)	22.3	13.4
D_m /g (mass loss) (STD)	4.5	6.0
D_m /g (mass loss) (CV%)	20	45
Overall statistics		
D_m (AVG)	487	466
D_m (STD)	29	16
D_m (CV%)	6	3
D_m /g (mass loss) (AVG)	22.1	15.8
D_m /g (mass loss) (STD)	4.1	7.1
D_m /g (mass loss) (CV%)	19	45

AVG: Average. STD: Standard deviation. CV%: Coefficient of variation.

Table B.1(d) Repeatability Using Products in a Single Laboratory

Material	E Foam ^a	Sh Fl 1 ^b	Fl Tile ^c	PP Crp ^d	Lens ^e	Sh Fl 2 ^f
25 kW/m ² , NF						
D_m (AVG)	134	266	178	543	333	483
D_m (STD)	8	9	9	15	17	93
D_m (CV%)	6	3	5	3	5	19
D_{10} (AVG)	111	264	170	521	202	396
D_{10} (STD)	5	9	13	12	25	33
D_{10} (CV%)	5	4	8	2	12	8
25 kW/m ² , F						
D_m (AVG)	29	143	97	340	94	476
D_m (STD)	6	8	37	29	6	20
D_m (CV%)	19	6	38	9	7	4
D_{10} (AVG)	25	121	91	269	72	344
D_{10} (STD)	4	7	37	17	5	15
D_{10} (CV%)	15	6	40	6	7	4
50 kW/m ² , F						
D_m (AVG)	125	304	144	388	110	691
D_m (STD)	7	15	10	31	8	37
D_m (CV%)	6	5	7	8	2	5
D_{10} (AVG)	90	205	118	245	77	418
D_{10} (STD)	5	9	9	20	7	15
D_{10} (CV%)	5	4	8	8	3	4

AVG: Average. STD: Standard deviation. CV%: Coefficient of variation.

^aBlended polymeric/rubber compound used as thermal insulation.

^bCommercial PVC floor covering with inorganic felt backing.

^cCommercial filled PVC floor tile.

^dCarpet with polypropylene yarn and scrim.

^ePolymeric material used to cover fluorescent light fixtures.

^fResidential unfilled PVC floor covering.

Annex C Interlaboratory Application

This annex is not a part of the requirements of this NFPA document but is included for informational purposes only.

C.1 Calibration of the Working Heat Flux Meter. The calibration of the heat flux meter should be checked whenever a recalibration of the apparatus is carried out by comparing the working heat flux meter to two instruments of the same type and similar range, and held as reference standards not to be used for any other purpose. One of the heat flux meter reference standards should be fully calibrated at an accredited laboratory at yearly intervals. This meter should be used to calibrate the heater temperature controller. [See Figure 4.3.2.1(a) and Figure 4.3.2.1(b).] The meter should be positioned at a location equivalent to the center of the specimen face during this calibration. One option for making the comparison of working and reference standard heat flux meters as required in 4.3.4.3

is the use of the conical heater (see 4.3.1), with each heat flux meter mounted in turn in the calibration position (see 4.3.1.2), taking care to allow the whole apparatus to attain thermal equilibrium. Alternatively, an apparatus specially built for comparative purposes can be used — for example, as described in BS 6809, *Method of Calibration of Radiometers for Use in Fire Testing*.

It is noted that the use of two reference instruments rather than one provides a greater safeguard against change in sensitivity of the reference instruments.

C.2 Variability in the Specific Optical Density of Smoke Measured in This Single-Chamber Test.

C.2.1 A preliminary interlaboratory trial has been carried out in which replicate batches of 16 materials were tested in accordance with this test method by eight laboratories in six countries. This preliminary interlaboratory trial showed that

the specific optical densities D_s (at 10 minutes) of some materials had a higher relative variability than those of others. The relative variability increased particularly for those materials that did not ignite readily at an incident heat flux of 25 kW/m², and for those materials that showed higher D_s (at 10 minutes) values in the nonflaming mode than in the flaming mode.

C.2.2 The preliminary interlaboratory trial has demonstrated the ability of this test apparatus to discriminate between materials that generate different levels of smoke. Table B.1(a) and Table B.1(b) present the repeatabilities and reproducibilities of D_s (at 10 minutes) for five plastics and five building materials, as derived in accordance with the statistical analysis in ISO 5725-1, *Accuracy (trueness and precision) of measurement methods and results — Part 1: General principles and definitions*, and ISO 5725-2, *Accuracy (trueness and precision) of measurement methods and results — Part 2: Basic method for the determination of repeatability and reproducibility of a standard measurement method*.

C.2.3 Repeatability, r , is the value below which the difference between two D_s (at 10 minutes) values obtained with the same method on identical test samples, under the same conditions (same laboratory, same apparatus, same operator, within a short interval of time), might be expected to be within a 95 percent probability.

C.2.4 Reproducibility, R , is the value below which the difference between two D_s (at 10 minutes) values obtained with the same method on an identical test sample, under different conditions (different laboratories, different operators, different apparatuses), might be expected to be within a 95 percent probability.

C.2.5 The preliminary interlaboratory trial suggests that it is not meaningful to quote a single value for the variability of the test. The D_s (at 10 minutes) data show that smoke generation depends on the ignition behavior of the materials (among other factors). Since ignition times are sensitive to irradiance (or incident heat flux), it is clear that careful attention should be paid to the measurement of irradiance.

C.2.6 A further examination of repeatability was also conducted in a single laboratory for wood samples, and the results are shown in Table B.1(c). It is clear from these results that the repeatability of the test method is much better if the materials tested undergo consistent ignition under the conditions used for testing.

C.2.7 Six different products were selected for evaluation in a single laboratory. These selections represent typical commercial products that display a wide range of responses when subjected to the heat fluxes and the ignition source employed in this test method. An analysis of the data was conducted as a measure of the repeatability of the test method. See Table B.1(d), which also identifies the products included in the study. The repeatability of the test method for this selection of products is good, as indicated by the calculated coefficient of variation, $CV\%$. Some of the products are difficult to ignite, some of them bulge toward the heater, and some of them melt; however, the combination of the cone heater and the horizontal orientation minimizes the effect of these common performance problems.

Annex D Determination of Mass Optical Density

This annex is not a part of the requirements of this NFPA document but is included for informational purposes only.

D.1 Introduction. The value of mass optical density determined by this test method is specific to the specimen in the form and thickness tested and is not to be considered an inherent or fundamental property.

D.1.1 Principles of the Test. The conditions of thermal exposure and of smoke collection are the same as those in the mandatory part of the test method. Additional mass loss measurements are conducted on the specimen during the test, so that a mass loss/time curve is determined and mass optical density can then be calculated.

D.1.2 Test Specimen. The same specifications on suitability of materials, products, or assemblies apply in this Annex as in the mandatory portion of the test method. (See Chapter 6.) Similarly, the same number of specimens, their preparation, and their conditioning also apply. (See Chapter 8.)

D.1.3 Ancillary Equipment.

D.1.3.1 The load cell should have a measuring range of 500 g and a weighing accuracy of ± 0.1 g. The load cell should be mounted in an enclosure [see Figure D.1.3.1(a) through Figure D.1.3.1(d)] with a close-fitting labyrinth seal between the sample support rod and the enclosure to minimize ingress of smoke particles and aggressive combustion products.

The load cell assembly should be easily removable from the smoke chamber, so that the mandatory test procedure can be performed without unnecessary exposure of the load cell, if mass optical density data are not required.

Figure D.1.3.1(a) through Figure D.1.3.1(d) differ from Figure 4.2.1, Figure 4.3.1.1, and Figure 4.3.2.1(a) in that they show the location of the (optional) load cell.

D.1.3.2 To level the unit on the base plate, the load cell enclosure should be fitted with one fixed foot and two adjustable feet. The load cell should also have a means to centralize the load cell assembly beneath the cone radiator.

D.1.3.3 The load cell should have a safe operating temperature range of 15°C to 70°C. A mineral fiberboard shield should be positioned over the top and sides of the load cell enclosure during thermal exposure of the test specimen, so that excessive temperature rise within the enclosure is prevented and drift of the load cell is avoided.

D.1.3.4 The load cell should be connected to a controller that drives the load cell and that is situated externally to the smoke chamber.

This controller preferably should be fitted with a digital mass display, a scalable millivolt output, and a sample tare facility.

D.1.4 Calibration Procedures. The load cell calibration should be checked with standard reference weights, in the range of test specimen mass, before each series of tests.

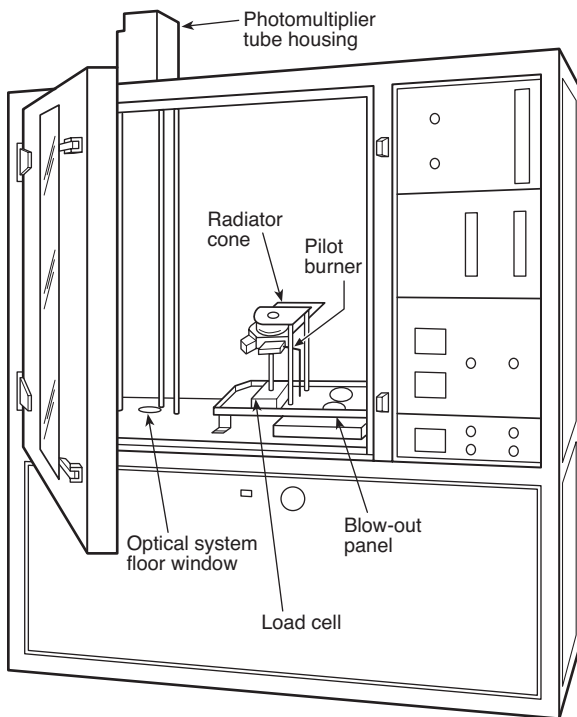


FIGURE D.1.3.1(a) Typical Arrangement of Test Chamber with Load Cell.

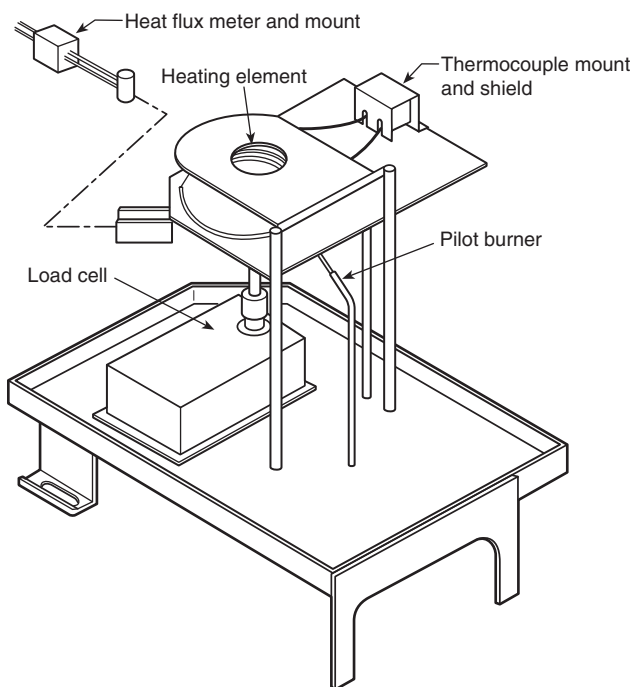


FIGURE D.1.3.1(b) Typical Framework for Support of Radiator Cone, Specimen, Flux Meter, and Load Cell.

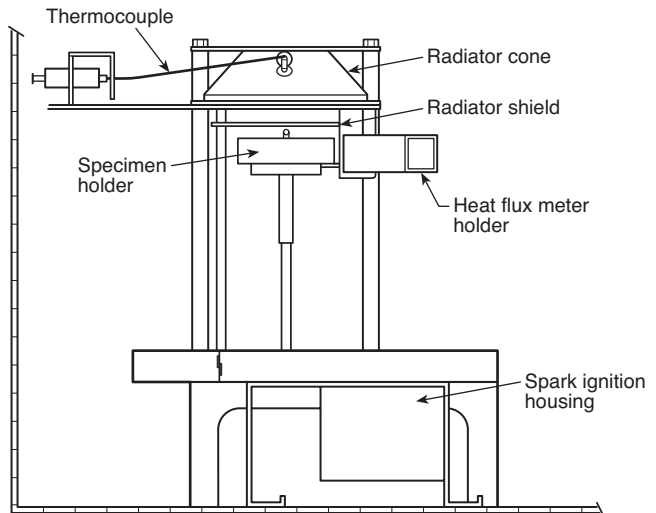


FIGURE D.1.3.1(c) Typical Arrangement of Radiator Cone, Specimen Holder, Radiator Shield, and Load Cell (side view), with Load Cell for Mass Optical Density Determination.

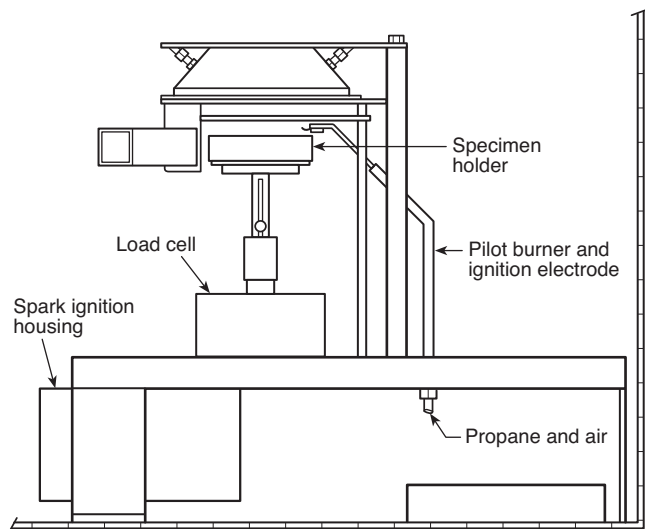


FIGURE D.1.3.1(d) Typical Arrangement of Radiator Cone, Specimen Holder, Radiator Shield, and Load Cell (front view).